



1
2
3
4
5
6
7

QIBA Profile. ¹⁸F-labeled PET tracers targeting Amyloid as an Imaging Biomarker

Version [with PUBLIC COMMENTS considered](#)

[15 June 2017](#) [02 May 2018](#)

Table of Contents

8

9 [1. Executive Summary](#) 6

10 [1.1 Overview](#) 6

11 [1.2 Summary for Clinical Trial Use](#) 7

12 [1.3 Intended Audiences](#) 8

13 [2. Clinical Context and Claims](#) 8

14 [2.1. Claim](#) 9

15 [2.2. Considerations for claim](#) 9

16 [2.3. Clinical Trial Utilization](#) 10

17 [3. Profile Activities](#) 16

18 [3.1. Subject Handling](#) 18

19 [3.2. Image Data Acquisition](#) 22

20 [3.3. Imaging Data Reconstruction and Post-Processing](#) 28

21 [3.4. Image Analysis](#) 34

22 [3.5. Image Interpretation and Reporting](#) 46

23 [3.6. Quality Control](#) 46

24 [4. Conformance Procedures](#) 56

25 [4.1. Performance Assessment: Image Acquisition Site](#) 56

26 [4.2. Performance Assessment: PET Acquisition Device](#) 57

27 [4.3. Performance Assessment: Reconstruction Software](#) 63

28 [4.3. Performance Assessment: Image Analysis Workstation](#) 65

29 [4.3. Performance Assessment: Software Version Tracking](#) 68

30 [References](#) 69

31 [Appendices](#) 78

32 [Appendix A: Acknowledgements and Attributions](#) 78

33 [Appendix B: Background Information for Claim](#) 80

34 [Appendix C: Conventions and Definitions](#) 83

35 [Appendix D: Model-specific Instructions and Parameters](#) 88

36 [Appendix E: Data fields to be recorded in the Common Data Format Mechanism](#) 91

37 [Appendix F: Testing PET Display and Analysis Systems with the UW-PET QIBA Amyloid Digital Reference](#)

38 [Object \(DRO\) Series](#) 92

39 [Appendix G: Best Practice Guidance for the Hoffman Brain Phantom](#) 97

40 [Appendix H: Detailed Example of Hoffman Phantom Data Analysis](#) 99

41	Method Overview	100
42	Relevant Data Files	100
43	Appendix I: Kinetic Modeling and Comparison to SUVR	117
44	1. Executive Summary	5
45	 Summary for Clinical Trial Use	5
46	2. Clinical Context and Claims	6
47	 Utilities and Endpoints for Clinical Trials	6
48	 Claim	7
49	3. Profile Activities	9
50	 3.1. Subject Handling	10
51	 3.2. Image Data Acquisition	14
52	 3.3. Imaging Data Reconstruction and Post-Processing	20
53	 3.4. Image Analysis	25
54	 3.5. Image Interpretation and Reporting	35
55	 3.6. Quality Control	36
56	4. Conformance Procedures	45
57	 4.1. Performance Assessment: Image Acquisition Site	45
58	 4.2. Performance Assessment: PET Acquisition Device	46
59	 4.3. Performance Assessment: Reconstruction Software	52
60	 4.4. Performance Assessment: Image Analysis Workstation	54
61	 4.5. Performance Assessment: Software version tracking	57
62	References	57
63	Appendices	61
64	 Appendix A: Acknowledgements and Attributions	61
65	 Appendix B: Background Information for Claim	63
66	 Appendix C: Conventions and Definitions	63
67	 Appendix D: Model-specific Instructions and Parameters	68
68	 Appendix E: Data fields to be recorded in the Common Data Format Mechanism	70
69	 Appendix F: Testing PET/CT Display and Analysis Systems with the FDG PET/CT Digital Reference Object	71
70	 Appendix G: Best Practice Guidance for the Hoffman Brain Phantom	76
71	 Appendix H: Detailed Example of Hoffman Phantom Data Analysis	78
72	Phantom Description	78

74	Methods and Metrics	79
75	Method Overview	79
76	Relevant Data Files	79
77	Method Details — Processing Steps	81
78	Example Results using the ADNI Hoffman Qualification Data	81
79		
80		

Open Issues:

The following open issues have been raised. They are provided here to capture the associated discussion, to focus the attention of reviewers on topics needing feedback, and to track them so they are ultimately resolved. Comments on these issues are highly encouraged during the Public Comment stage. This version incorporates text to address public comments received in response to the version of the Profile dated June 2017.

~~Claim Context~~ Modifications to address public comments

If and how to address concern that large (>8% change in SUVR across time) may be accounted for by biologic change unrelated to amyloid deposition difference alone. Modifications have been incorporated to address public comment and issues that were outstanding, including the Claim(s). These are subject to additional review.

Conformance Methodology

The methodology to perform conformance testing of the image analysis workstation is included; this relies upon using a Digital Reference Object (DRO), which ~~is still a work in progress~~ is in the process of being completed, funded as a NIBIB groundwork project.

~~Region Segmentation Requirements~~

If and how to define requirements around anatomic region segmentation (whether anatomic specific to a subject (e.g. MRI-PET fused) or atlas based)) across time which may or may not be radiotracer dependent.

Conformance Testing

Need to describe a study that actors need to perform to test that: ~~1-1) Their wCV is~~ within the parameter stated in the Claim ~~<0.029, 2-1, 2) hat the wCV is constant over~~ the a prescribed range of SUVRs and 3-1, and 3) hat linearity with a slope of one is a reasonable assumption.

References

Literature references are incomplete. These will be completed during the Public Comment phase.

1. Executive Summary

1.1 Overview

This QIBA Profile documents specifications and requirements to provide comparability and consistency for the use of PET imaging using 18F labeled tracers ~~which target amyloid across scanners in neurology~~ that bind to fibrillar amyloid in the brain. Quantitative measurement of amyloid, a hallmark pathology of Alzheimer’s disease, has become increasingly used in clinical trials for patient inclusion, evaluation of disease progression, and assessment of treatment effects.

The Profile focuses on the use of Standardized Uptake Value Ratios (SUVRs) to measure amyloid burden, while also describing benefits associated with the Distribution Volume Ratio (DVR) (kinetic modeling) approach. The SUVR is determined using data acquired during a time window following a certain time period after tracer injection that is intended to allow the tracer to reach “pseudo” equilibrium. This approach has practical advantages, particularly for multi-site studies, due to the reduced time required for the patient to be in the scanner (and for older scanners, the lesser amount of data acquired for a single scan).

The guidance in this Profile can be applied for clinical trial use as well as individual patient management.

The document primarily addresses PET/CT imaging; however, a dedicated PET that has transmission capabilities can also be used. PET/MR scanners are not strictly excluded in this version as long as the repeatability of the SUVRs from these scanners is conformant with the assumptions underlying the claims.

~~PET/MR scanners are excluded in this version because of their novelty and unknown quantification differences as compared to PET/CT and dedicated PET scanners. The guidance in this Profile can be applied for both clinical trial use as well as individual patient management. This document organizes acquisition, reconstruction and post-processing, analysis and interpretation as steps in a pipeline that transforms data to information to knowledge.~~

~~The document~~This Profile, developed through the efforts of the amyloid Profile writing group in the QIBA Nuclear Medicine Technical Subcommittee, ~~has shared~~shares some content with the QIBA FDG-PET Profile, ~~as well as~~and includes additional material focused on the devices and processes used to acquire and analyze amyloid tracer PET data. The Profile is organized as follows:

Formatted: English (United States)

Formatted: Font: 11.5 pt, Font color: Custom Color(RGB(33,33,33)), Pattern: Clear (Bright Green)

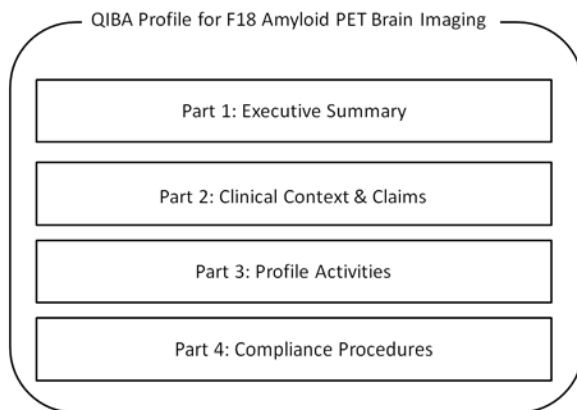


Figure 1: Illustration of the Profile components

The Profile Part 3 is derived from multiple sources, including material contained in the work performed by the Alzheimer's Disease Neuroimaging Initiative (ADNI). The current version of the Profile focuses on a longitudinal Claim, where the primary purpose is to assess change in amyloid load due to disease or following an intervention. In this case, precision is most important as long as bias remains constant over time. A high level of image measurement precisionCharacterization of measurement bias may be most will be important for a cross-sectional Claim wherein the amyloid tracer is used primarily to select amyloid positive subjects. For the current Profile, which is a longitudinal Claim, the primary purpose is to assess for change in amyloid load following an intervention; precision may be more important than bias as long as bias remains constant over time.

1.2 Summary for Clinical Trial Use

The QIBA Amyloid-PET Profile defines the technical and behavioral performance levels and quality control specifications for brain amyloid tracer PET scans used in single- and multi-center clinical trials of neurologic disease, primarily dementiaparticularly Alzheimer's disease. The specific claims for accuracyExamples of clinical application are detailed below in the Claims.

The aim of the QIBA Profile specifications is to minimize intra- and inter-subject, intra- and inter-platform, and inter-institutional variability of quantitative scan data due to factors other than the intervention under investigation. PET studies using an amyloid tracer, performed according to the technical specifications of this QIBA Profile provides qualitative and/or quantitative data for multi-time point comparative assessments (e.g., response assessment, investigation of predictive and/or prognostic biomarkers of treatment efficacy). While the Profile details also apply to studies assessing subjects at a single time point, a cross-sectional Claim is not currently included in this Profile.

A motivation for the development of this Profile is that while a typical PET scanner measurement system (including all supporting devices) may be stable over days or weeks; this stability cannot be expected over the time that it takes to complete a clinical trial. In addition, there are well known differences between scanners and/or the operation of the same type of scanner at different imaging sites. Particularly for longitudinal studies, precise quality control of the scanner both daily and periodically for stability is of paramount relevance. In addition, a process of harmonization is also of high relevance to make results

comparable between centers.

1.3 Intended Audiences

Formatted: English (United States)

The intended audiences of this document include:

- Technical staff of software and device manufacturers who create products for this purpose.
- Biopharmaceutical companies, neurologists, and clinical trial scientists designing trials with imaging endpoints.
- Clinical research professionals.
- Radiologists, nuclear medicine physicians, technologists, physicists and administrators at healthcare institutions considering specifications for procuring new ~~PET/CT (or PET/MR in subsequent document versions)~~ equipment for PET imaging.
- Radiologists, nuclear medicine physicians, technologists, and physicists designing PET/CT (and PET/MR) acquisition protocols.
- Radiologists, nuclear medicine physicians, and other physicians or physicists making quantitative measurements from PET images.
- Regulators, nuclear medicine physicians, neurologists, and others making decisions based on quantitative image measurements.

Note that specifications stated as 'requirements' in this document are only requirements to achieve the claim, not 'requirements for standard of care.' Specifically, meeting the goals of this Profile is secondary to properly caring for the patient.

2. Clinical Context and Claims

Accumulation of amyloid-B (AB) fibrils in the form of amyloid plaques in the brain is a ~~neuropathological~~ requirement for the pathologic diagnosis of dementia due to Alzheimer's disease (AD). Among the various biomarkers in development to assess AB, 18F PET amyloid radiotracers (see Table in Section 3.1.3.1.2 ~~of for~~ currently approved ~~radiotracers for qualitative amyloid burden assessment which~~) offer the potential of directly detecting and quantifying ~~cortical AB deposition~~ amyloid burden. Amyloid quantitation is being used to determine whether levels exceed a threshold for positivity (a cross sectional application) for patient inclusion in clinical trials and to measure changes in amyloid burden over time (a longitudinal application) to assess disease progression or modification by therapeutic intervention. ~~The rationale for their use in neurology is based on the typically increased presence of cortical AB deposition in individuals with mild cognitive impairment (MCI) due to AD and AD compared to normal control subjects without amyloid deposition.~~

Utilities and Endpoints for Clinical Utility

Formatted: Normal

~~B-amyloid (AB) imaging with PET permits in vivo assessment of AB deposition in the brain.~~

Formatted: Left

This QIBA Profile ~~specifically~~ addresses the requirements for measurement of 18F- amyloid tracer uptake with PET as an imaging biomarker for assessing the within subject change in brain amyloid burden over time (longitudinal Claim) to inform the assessment of disease status or ~~possibly~~ to evaluate therapeutic drug response. ~~Quantitative assessment of amyloid burden at a single time point (cross-sectional or bias Claim) is not part of the current Profile.~~

Biomarkers useful in clinical research for patient stratification or evaluation of therapeutic response would be useful subsequently in clinical practice for the analogous purposes of initial choice of therapy and then potential future clinical use is also in the individualization of therapeutic regimen based on the extent and degree of response as quantified by amyloid-PET. Quantitative assessment of amyloid burden at a single time point (cross sectional or bias Claim) is not part of the current Profile but may be included in a future version as bias reference data becomes available.

Formatted: Left

The technical specifications described in the Profile are appropriate for measuring longitudinal changes within subjects. Portions of the Amyloid PET Profile details are drawn from the FDG-PET Profile and are generally applicable to quantitative PET imaging for other tracers and in other applications.

A negative amyloid PET scan indicates sparse to no neuritic plaques and a positive amyloid scan indicates moderate to frequent amyloid neuritic plaques.

2.1. Claim

Formatted: English (United States)

If Profile criteria are met, then:

Formatted: Space After: 0 pt

Claim 1: Brain amyloid burden as reflected by the SUVR is measurable from 18F amyloid tracer PET with a within-subject coefficient of variation (wCV) of $\leq 1.94\%$.

Formatted: Justified, Space After: 0 pt

Formatted: Font: Segoe UI, 11.5 pt

This technical performance claim is to be interpreted in the context of the considerations stated below.

Formatted: Justified, None, Space After: 0 pt

Formatted: Font: (Default) Segoe UI, 11.5 pt, Font color: Auto

2.2. Considerations for claim

Formatted: English (United States)

The following important considerations are noted:

Formatted: Justified, None, Space After: 0 pt

1. The technical performance claim was derived from a review of the literature summarized in Appendix B, where 18F amyloid PET tracers were used and data acquisition and processing procedures were considered to be adequately aligned with the recommendations in this profile. The constraint of a sixty day period (or less) for test-retest was applied in order to avoid the possible contribution of actual changes in amyloid burden. The wCV cited is the highest ("worst case") of these short term test-retest studies, where wCV values ranged from 1.15% in healthy controls using a cerebellar cortex reference region to 1.94% in AD patients using a whole cerebellum reference region. A limitation is that only two relatively small studies covering three study groups (2 AD, 1 healthy control) satisfied the short term test-retest criteria and were aligned with profile recommendations. Given this limitation, and in order to assess the applicability of the short term wCV reference for typical clinical trial durations, the wCV values derived from two studies of amyloid negative normal controls from the larger ADNI data set over a 2 year period, using a variety of reference regions, were examined. The wCV values in these longer term studies ranged from 1.25% (white matter reference region) to 1.6% (whole cerebellum reference region) in four of five cases, within the range stated by the claim. For the same set of images, the wCV in one group's analysis was 3.38% for one reference region vs. 1.37% for another. The important consideration of analysis methods is discussed in consideration number 2. The reference

Formatted: Justified, None, Indent Left: 0", Hanging: 0.31", Space Before: 6 pt, After: 0 pt

literature is discussed further in [Appendix B](#).

2. [Conformance to the Claim depends upon many factors, including minimized subject motion, alignment of Em/Tx scans, and stability in detection sensitivity from scan to scan in reference region slices compared to target region slices. In particular, choice of reference region, and the boundary definition of the reference region selected can greatly impact wCV due to the sensitivity of different regions to technical factors. A more extensive discussion of the considerations in selecting reference region is found in section 3.4.3.2.2.](#)
3. [This Claim is applicable for single or multi-center studies assuming that the same 18F-amyloid PET tracer, scanner, scanner software version, image acquisition parameters, image reconstruction method and parameters, and image processing methods including target and reference region definition and boundaries are used for each subject at each time point as described in the Profile.](#)
4. [It is presumed that a\) the wCV is constant over the range of SUVR values and b\) any bias in the measurements is constant over the range of SUVR values \(linearity\). \(The assumption of linearity and its demonstration are discussed further in section 4.4 and Appendix F.\)](#)
5. [The SUVR has been selected due to its logistical feasibility in multi-site trials, and its use to date in large reference studies such as ADNI. However, from the fundamental kinetic properties of radiotracers it can be understood that changes in SUVR may not represent only a change in specific signal \(amyloid\) but could, at least in part, be the result of changes or variability in perfusion \(van Berckel et al, J Nucl Med. 2013\) and/or tissue clearance \(Carson RE et al, 1993\). When random, this variability contributes to and is embedded in the wCV stated in the Claim. However, changes in perfusion and/or clearance can be systematic due to the action of certain pharmacological agents or due to disease progression, creating artificial change in amyloid SUVR. A published study using ADNI data suggests that the impact of regional cerebral blood flow changes on longitudinal change in SUVR can be on the order of 2% to 5% in late MCI/AD patients \(Cselényi\). This can be significant in studies of amyloid accumulation, prevention, or modest amyloid removal.](#)

[Whether or not a change in SUVR is affected by changes in perfusion and/or clearance ideally should be first demonstrated in a small \(e.g. 20 subjects\) cohort before SUVR is used in the larger clinical trial. These contributions can be quantified by applying kinetic modeling to a full image acquisition from time of tracer injection through late timeframes. These validation studies can help to assess the minimally required decrease in SUVR that is needed to rule out false positive findings because of disease and/or drug related perfusion effects. Alternate approaches to assessing blood flow changes have also been proposed \(e.g. arterial spin labeling MRI\) though suitability remains to be validated. As a separate consideration, in the case of a new PET tracer, studies that include blood sampling should be conducted to confirm that the SUVR approach and use of a reference region are a suitable approach to measure tracer binding. For further details regarding considerations in kinetic modeling and a comparison to SUVR please see Appendix I.](#)

2.3. Clinical Trial Utilization

[Although the Claim is based on reference literature for a short duration, as suggested by the 2 year comparison studies, the wCV should apply longer term pending the stated considerations.](#)

Formatted: Justified, None, Space After: 0 pt

Formatted: English (United States)

Formatted: Justified, Space After: 0 pt

The wCV stated in the technical performance Claim can be used to derive confidence intervals for individual subject changes in amyloid burden. However, because amyloid accumulation rates reported in the literature average from 1 percent to a few percent per year, SUVR confidence intervals derived from the wCV may not be relevant to the assessment of individual change over the duration of a typical clinical trial. In this case, the wCV value can be used to guide the number of subjects to include in clinical trials targeting measurement of longitudinal change in amyloid SUVR. A few examples of practical uses of the Claim are described below, and further guidance is found in the “Statistical Planning for a Clinical Trial Guidance document” posted on the QIBA website, in development as a full manuscript.

1. Powering a clinical trial to measure rate of amyloid accumulation. As an example, suppose you want to estimate the mean amount of amyloid accumulation in a two-year period for a cohort of patients. You want to estimate the mean amount of accumulation to within +1% (i.e. precision of 95% CI). We considered mean SUVR values at baseline from 1.0-1.5, between-subject standard deviation (SD B) ranging from 0.05 to 0.30, and correlation between the paired measurements from a subject of $r=0.3$ (first figure panel), 0.5 (second panel), and 0.9 (third panel). The figure shows the number of subjects needed if the likely rate of amyloid accumulation is 1.5% per year.


Formatted: Font: Bold
Formatted: Normal, Justified, Indent: Left: -0.06", Hanging: 0.31", Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"



Formatted: Justified, Indent: Left: 0", Space After: 0 pt
Formatted: Justified, Indent: Left: 0.25", Space After: 0 pt

Formatted: Justified, Space After: 0 pt
Formatted: Normal, Centered, Indent: Left: 0"

Formatted: Normal, Justified, Indent: Left: 0"

Note that the number of subjects required is greatly reduced as the correlation coefficient increases between visits. For context, an internal (unpublished) analysis of florbetapir data available through ADNI at baseline and 2 years suggests that the correlation between scans is higher for certain reference regions than others. For example, using the composite of cerebellum and white matter or only white matter as reference, R was 0.95 or 0.96 respectively for amyloid positive subjects (N=207) and 0.94 for subjects close to the positivity threshold (N=51). However, using cerebellar cortex or whole cerebellum as the reference, R values were 0.79 and 0.83 respectively for amyloid positive subjects and 0.33 and 0.48 respectively for subjects close to positivity threshold.

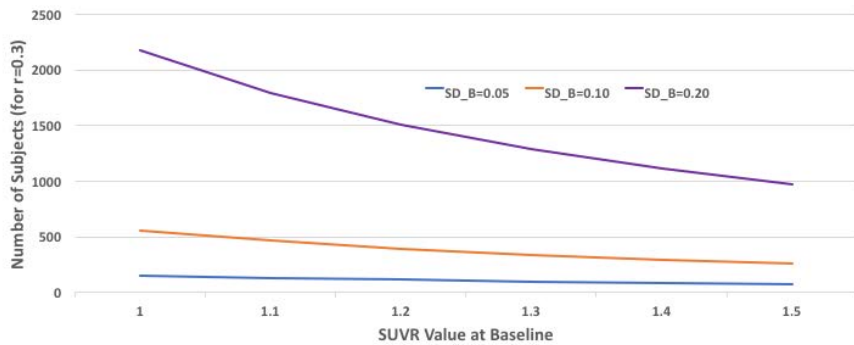

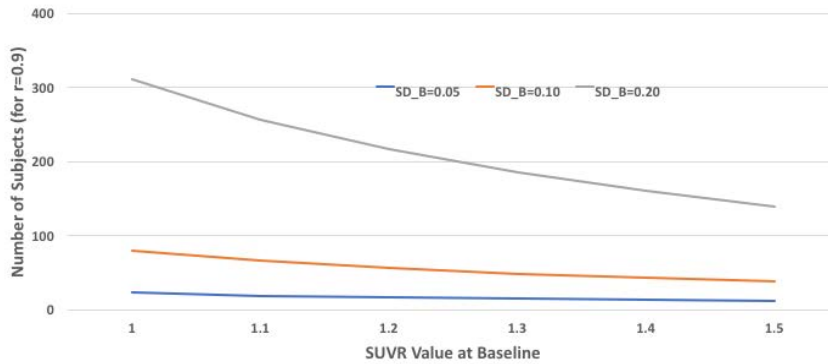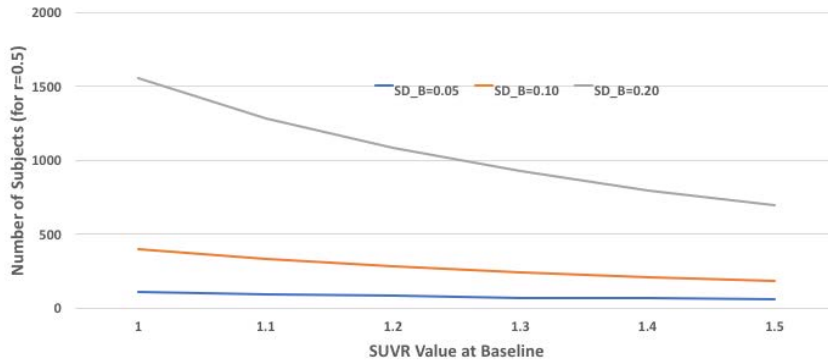

Formatted: Normal, Centered, Indent: Left: 0", Widow/Orphan control


Formatted: Normal, Justified, Indent: Left: 0", Widow/Orphan control

Formatted: Font: Bold

Formatted: Normal, Justified, Indent: Left: -0.13", Hanging: 0.38", Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

Formatted: Normal, Justified, Indent: Left: 0"

2. **Powering a clinical trial to measure a reduction in the rate of amyloid accumulation (e.g. due to treatment intervention).** Consider a clinical trial comparing the accumulation in amyloid SUVR over time between two groups of subjects: those undergoing a new treatment vs. a control group. Alzheimer's patients will be recruited and randomized to either the experimental intervention or the control group. SUVR will be measured in all subjects at baseline and two years later. The null hypothesis is that there is no difference in subjects' mean amyloid accumulation between the two groups; the alternative hypothesis is that there is a difference (two-tailed hypothesis). If the likely rate of amyloid accumulation is 1.5% per year, the mean SUVR at baseline is 1.5, the between-subject standard deviation is between 0.05 and 0.2, and the correlation between the paired measurements from a subject is between 0.3 and 0.9, then the following figure illustrates the number of subjects needed per arm to detect a 50% reduction in the rate of accumulation over a 2-year period with 80% power.

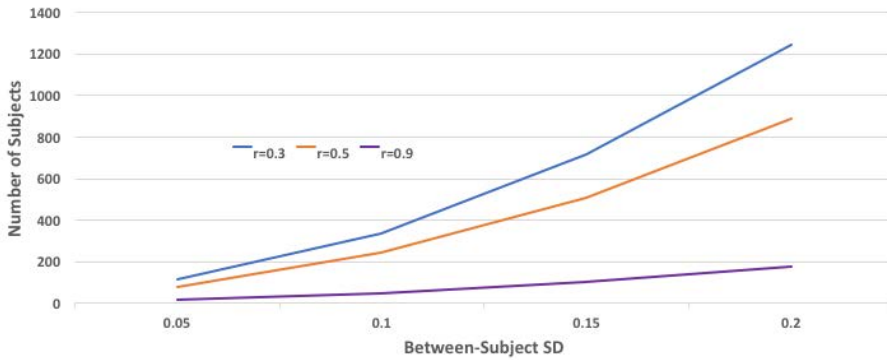

Formatted: Normal, Centered, Indent: Left: 0"


315
316
317 **3. Minimum detectable Increase for individual subject.** The smallest increase in SUVR that can
318 be considered a real increase in amyloid accumulation for an individual subject (not just
319 measurement error), with a certain confidence level, can be calculated as: $Y1 \times (0.0194) \times \sqrt{2} \times$
320 $(z - \text{value})$. The figure shows the minimum detectable increase for 70%, 80%, 90%, and 95%
321 confidence for baseline SUVR values from 0.5-2.0.

Formatted: Normal, Justified, Indent: Left: 0"

Formatted: Font: Bold

Formatted: Justified, Indent: Left: 0", Space After: 0 pt

Formatted: Font: Italic

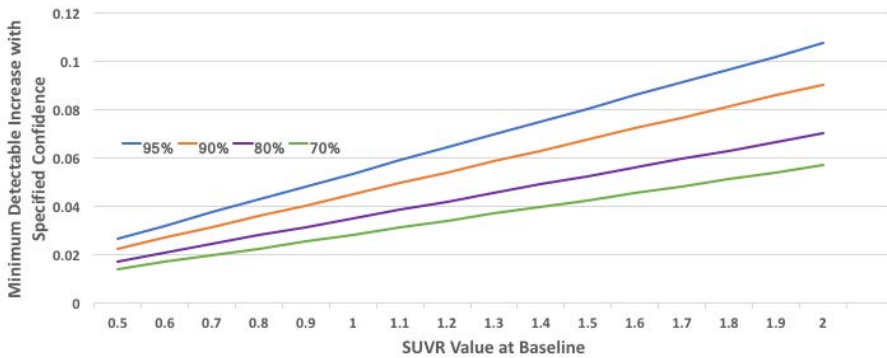

Formatted: Centered, Indent: First line: 0", Space After: 0 pt

322
323
324 **4. Confidence interval for an individual's true change.** For an individual's SUVR measurements of Y1 at
325 baseline and Y2 at follow-up, the 95% confidence interval for the true change associated with the wCV
326 of Claim 1 is given by the equation: $(Y2-Y1) \pm 1.96 \times \sqrt{([Y1 \times 0.0194]^2 + [Y2 \times 0.0194]^2)}$.

Formatted: Justified, Indent: First line: 0", Space After: 0 pt

Formatted: Justified, Indent: Left: 0", Space After: 0 pt

Formatted: Font: Bold

Formatted: Justified, Space After: 0 pt

Formatted: Space After: 0 pt

Claim:

If Profile criteria are met, then:

Claim 1: Brain amyloid burden as reflected by the SUVR is measurable from 18F amyloid tracer PET with a within-subject coefficient of variation of 2.9%

Claim 2: A measured change in SUVR of Δ % indicates that a true change has occurred if $\Delta > 8$ %, with 95% confidence.

Claim 3: If Y1 and Y2 are the SUVR measurements at two time points, then the 95% confidence interval for the true change is $(Y2 - Y1) \pm 1.96 \times \sqrt{[(Y1 \times 0.029]^2 + [Y2 \times 0.029]^2}$.

This Profile's Claims have been informed by an extensive review of the literature (See Appendix B), including a meta-analysis that was performed as part of the groundwork effort; however, it is currently a consensus claim that has not yet been substantiated by studies that strictly conform to the specifications in this document. The Committee recognizes that the threshold change metric (8%) currently cited in the Claim may not be practical or relevant for the assessment of biologic change or a modification of biologic change with a therapeutic intervention, since accumulation rates reported in the literature are on average from 1% to a few percent per year. However, the cited threshold must be supported by relevant test-retest literature. The reference test-retest studies that were used to determine the threshold were limited to those meeting a test-retest time window of 60 days or less. However, these studies did not necessarily incorporate the approaches to limit variability that are recommended in this Profile. While more recently published and unpublished studies have suggested tighter tolerances when factors such as reference region are optimized, those studies did not meet the test-retest duration criterion of 60 days or less. Despite these limitations, it is the Committee's opinion that by sharing the outlined performance requirements contained herein, the community of professionals using amyloid imaging in both clinical trials and clinical practice will be able to obtain more robust data which can then refine the Claim thresholds.

The following important considerations are noted:

1. This Claim applies only to subject scans that are considered evaluable with PET. In practice this means that scans are of sufficient diagnostic quality and performed with appropriate analysis requirements such that the target and reference tissue ROIs are evaluable. More details on which subject's scans are evaluable are described in Section 3.6.5.3.

2. Details of the claim were derived from a review of the literature and are summarized in Appendix B. In these reports, it was assumed that the repeatability of SUVR could be described.

3. This Claim is applicable for single-center studies using the same scanner model (and release). For multi-center studies, if 18F amyloid tracer PET imaging is performed using the same scanner and protocol for each subject at each time point (as described in the Profile), then it is anticipated that this Claim will be met.

4. For this longitudinal Claim the percent change in SUVR is defined as $\frac{(\text{SUVR at Time Point 2} - \text{SUVR at Time Point 1})}{\text{SUVR at Time Point 1}} \times 100$.

5. The statistical metric for Claim 1 is the Repeatability Coefficient (RC) and the statistical metric for Claim 2 is the within-subject coefficient of variation.

6. For both Claims, it is presumed that a) the wCV is constant over the range of SUVR values and b) any bias in the measurements is constant over the range of SUVR values (linearity).

7. In this Profile, SUVR will be measured using pixel counts or SUVmean of the target regions of interest normalized to that of a reference region. As SUVR simply represents the target to reference ratio, reconstructed images do not need to be converted to SUV images prior to SUVR calculation (See Figure 3 legend). SUV is a simplified metric representing the radiotracer uptake at a prescribed uptake time interval post injection. SUV is a composite signal consisting of contributions from radioactivity present in tissue arising from tracer signal in blood (typically 3-8% of tissue consists of blood volume), the tracer free, non-specifically and/or non-selectively bound in tissue and the tracer specifically bound to a target of interest, in this case amyloid (Gunn RN et al. JCBFM. 2001 Jun;21(6):635-52, Innis et al, JCBFM. 2007 Sep;27(9):1533-9, Schmidt KC³, Turkheimer FE, Q J Nucl Med. 2002 Mar;46(1):70-85.) . By normalising SUV to that of a reference region a simplified metric for the distribution volume ratio (DVR) is derived attempting to cancel or compensate for the contributions from the free and non-specifically bound tracer in tissue. However, the absolute signals and relative contributions arising from the various compartments are uptake time dependent as a result of differences in perfusion and non-specific and specific binding across the brain. In particular, it should be noted that perfusion does not only determine the wash-in (delivery) of the tracer, but also the wash-out of the tracer. Moreover, the wash-out is affected by the relative contributions of non-specific and specific binding as well, i.e., more 'binding slows down' wash-out. The latter also explaining the upward bias seen in SUVR compared with DVR (van Berckel et al, J Nucl Med. 2013 Sep;54(9):1570-6). A detailed discussion on the various sources of bias when using the simplified reference tissue model (and SUVR) can be found in (Salinas et al. JCBFM Feb;35(2):304-11, 2015). From the fundamental kinetic properties of radiotracers it can be understood that both SUV and SUVR (as surrogate for DVR) are perfusion dependent and that changes in perfusion across the brain as well as longitudinally will result in changes in SUVR. Consequently, changes in SUVR may not represent only a change in specific signal (amyloid) but could, at least in part, be the result of changes or variability in perfusion (van Berckel et al, J Nucl Med. 2013 Sep;54(9):1570-6) and/or tissue clearance (Carson RE, Channing MA, Blasberg RG, Dunn BB, Cohen RM, Rice KC, Herscovitch P. Comparison of bolus and infusion methods for receptor quantitation: application to [18F]cyclofoxy and positron emission tomography. J Cereb Blood Flow Metab. 1993 Jan;13(1):24-42). Whether or not a change in SUVR is affected by changes in amyloid and/or perfusion ideally should be first demonstrated in a small cohort before SUVR is used in the larger clinical trial. At the very least these validation studies should be performed to assess the minimally required decrease in SUVR that is needed to rule out false positive findings because of (disease and/or drug related) perfusion effects.

In addition, this claim should be re-assessed for technology changes, such as PSF (point spread function) based reconstruction or TOF (time of flight) imaging that were not utilized in published test-retest studies. A standard utilized by a sufficient number of studies does not exist to date. The expectation is that from future studies and/or field testing, data will be collected and changes made to this Claim or the Profile specifications accordingly.

3. Profile Activities

The following figure provides a graphical depiction that describes the marker at a technical level. The resulting SUVR measure of amyloid burden is then interpreted per the thresholds and/or other criteria determined per the study (this differs from visual interpretation).

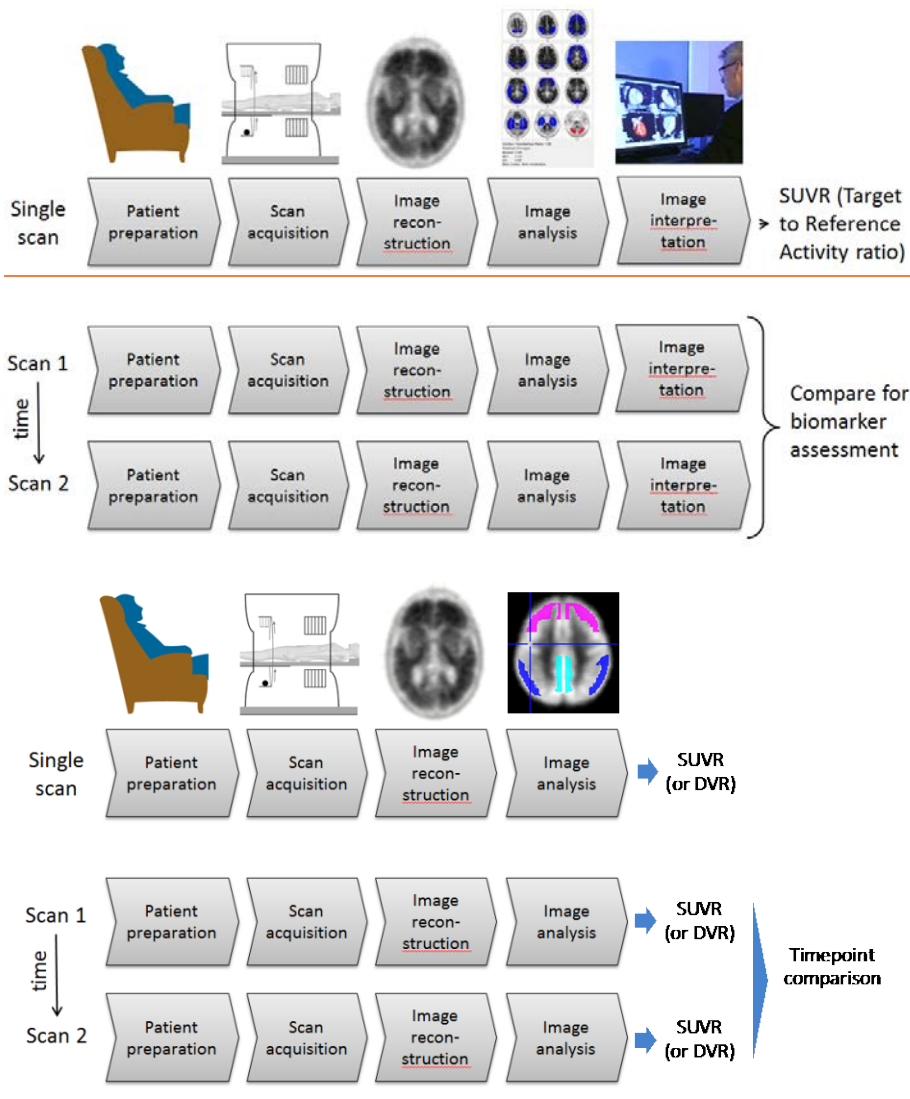


Figure 3: The method for computing and interpreting brain amyloid burden using PET may be viewed as a series of steps using either one scan (corresponding to a fit for use of a future ‘Cross-sectional’ Claim) or two or more scan sequences or time points (corresponding to a fit for use of the current Profile’s ‘Longitudinal’ Claim). For a given scan, the SUVR represents the ratio of tissue concentration for a designated brain region (or composite regions) compared to the activity from a reference region (which has typically been cerebellum (whole or gray) or pons but may involve other regions— see Section 4.4). The ratio of concentration from these distinct regions (target/reference) is then calculated, which is termed the SUVR.

Furthermore, as discussed in the Image Analysis Section of this Profile, the *Centiloid Scale* may, after further investigation, provide a mechanism whereby a study can be performed with different amyloid PET tracers and/or different processing pipelines or measurement methods mapped to a standard which is then comparable (e.g., by using a linear scaling process and looking at mean values [See Section 3.4.3.3.3]) to some (to be defined) degree range of numeric SUVR values (Klunk et al, 2015). At this time, pending validation of the centiloid methodology continues to undergo adoption and is not included in Profile requirements; this Further, this Profile requires the use of a single radiotracer in a multi-center trial presuming when pooling of data across centers is performed. For further description see section 3.4.3.3.3 of this Profile.

Patients may be selected or referred for amyloid-PET imaging through a variety of mechanisms.

The imaging steps corresponding to Figure 1 are:

- 1) Patients or subjects are prepared for scanning. The amyloid tracer is administered. Patient waits for bio-distribution and uptake of amyloid tracer. See Section 3.1.3.1.2 for ligand-specified timing.
- 2) Emission and transmission data are acquired (typically the PET scan and CT scan if a PET-CT scanner).
- 3) Data correction terms are estimated and the attenuation and scatter corrected images are reconstructed.
- 4) Images are assessed for quality control, and may separately be reviewed visually for qualitative interpretation (outside of the scope of this profile).
- 5) Quantitative (and/or semi-quantitative) measurements are performed.

Note that steps 4 and 5 may occur in either order or at the same time, depending upon the context of the review (clinical research versus clinical practice) with reference to the specifications described in each tracer’s package insert. Currently, the quantitative use of amyloid-PET tracers is not approved by any regulatory authorities in clinical practice in the U.S. However, quantitation is available as part of various scanner and workstation software packages and is used extensively in clinical trials. More details on the requirements are given below.

Images may be obtained at a single time point or multiple time points over months or years, for example at a minimum of two time points before and after therapeutic intervention for a response assessment.

The following sections describe the major components illustrated in Figure 3:

Section	Title	Performed by
3.1	Subject Handling	Personnel, (including Technologists and Schedulers) at an Image Acquisition Facility

Section	Title	Performed by
3.2	Image Data Acquisition	Technologist, at an Image Acquisition Facility using an Acquisition Device
3.3	Image Data Reconstruction	Technologist, at an Image Acquisition Facility using Reconstruction Software
3.4	Image Analysis	Imaging Physician or Image Analyst Radiologist, Nuclear Medicine Physician, Image Analyst, or other qualified person with the necessary training to using-use one or more <u>image Processing and Analysis Software</u> tools
3.5	Image Interpretation	Imaging Physician Radiologist, Nuclear Medicine Physician, or an individual <u>meeting requirements designated for the study; note that qualitative image interpretation is not within the scope of this Profile before or after information obtained by Image Analysis using a pre-defined Response Assessment Criteria</u>

450 Image data acquisition, reconstruction and post-processing are considered to address the collection and
 451 structuring of new data from the subject. Image analysis is primarily considered to be a computational step
 452 that transforms the data into information, extracting important values. Interpretation is primarily
 453 considered to be judgment that transforms the information into knowledge.

455 3.1. Subject Handling

456 This Profile will refer primarily to 'subjects', keeping in mind that the recommendations apply to patients in
 457 general, and that subjects are often patients too.

458 3.1.1 Subject Selection and Timing

459 The utility of correlative anatomic brain imaging, CT or MRI, can be viewed in two different contexts. From
 460 a clinical perspective, the anatomic imaging study is used to assess for evidence of bleed, infection,
 461 infarction, or other focal lesions (e.g., in the evaluation of subjects with dementia, the identification of
 462 multiple lacunar infarcts or lacunar infarcts in a critical memory structure may be important). From the
 463 perspective of establishing performance requirements for quantitative amyloid PET imaging, the purpose of
 464 anatomic imaging (separate from the utility of providing an attenuation correction map) is to provide
 465 assessment of cortical atrophy and consequently a falsely decreased SUVR. The image analyst should also
 466 be aware of the possibility of falsely increased SUVR due to blood-brain barrier (BBB) breakdown, such as in
 467 the case of intracranial bleed. The effect of differential BBB integrity inter-time point is currently not
 468 quantified in the scientific literature. While the performance of anatomic imaging is not a performance
 469 requirement of the Profile, the value of performing such imaging and the incorporation of its analysis with
 470 the amyloid PET findings may provide additional value in the interpretation for an individual subject. This
 471 should be considered in the design and implementation of the study protocol.

472 Aside from the exclusion (absolute or relative contraindications) of subjects who are unable to remain still
 473 enough to obtain adequate imaging (See Section 3.1.2.3 for information on subject sedation), subject
 474 selection for amyloid PET imaging is an issue beyond the scope of this Profile. Guidance for the use of
 475 amyloid to support diagnosis of symptomatic patients has been published in "Refer to Appropriate Use
 476 Criteria for Amyloid PET: A Report of the Amyloid Imaging Task Force". Asymptomatic or other clinical trials
 477 are guided by study objectives. See tracer, the Society of Nuclear Medicine and Molecular Imaging, and the

478 ~~Alzheimer's Association and~~ manufacturer guidance for ~~more additional~~ information regarding patient
479 ~~selection~~exclusions.

480 **3.1.1.1 Timing of Imaging Test Relative to Intervention Activity**

481 The study protocol should specifically define an acceptable time interval that should separate the
482 performance of the amyloid tracer PET scan from both (1) the index intervention (e.g., treatment with an
483 amyloid reducing therapeutic agent) and (2) other interventions (e.g., prior treatment). This initial scan (or
484 time point) is referred to as the "baseline" scan (or time point). The time interval between the baseline
485 scan and the initiation of treatment should be specified as well as the time intervals between subsequent
486 amyloid PET studies and cycles of treatment. Additionally, the study protocol should specifically define an
487 acceptable timing variance for acquisition of the amyloid PET scan around each time point at which imaging
488 is specified (i.e., the acceptable window of time during which the imaging may be obtained "on schedule").

489 **3.1.1.2. Timing Relative to Confounding Activities**

490 There are no identified activities, tests or interventions that might increase the chance for false positive
491 and/or false negative amyloid tracer PET studies which need to be avoided prior to scanning.

492 **3.1.1.3. Timing Relative to Ancillary Testing**

493 Various neuropsychiatric tests may be performed on or around the day of amyloid tracer imaging and
494 should be coordinated at the time of scheduling.

495 **3.1.2 Subject Preparation**

496 Management of the subject can be considered in terms of three distinct time intervals (1) prior to the
497 imaging session (prior to arrival and upon arrival), (2) during the imaging session and (3) post imaging
498 session completion. The pre-imaging session issues are contained in this section while the intra-imaging
499 issues are contained in section 3.2.1 on image data acquisition.

500 **3.1.2.1. Prior to Arrival**

501 There are no dietary or hydration requirements or exclusions.

502 The conformance issues around these parameters are dependent upon adequate communication and
503 oversight of the Scheduler or Technologist at the Image Acquisition Facility with the subject.
504 Communication with the subject and confirmation of conformance should be documented.

505 **3.1.2.2. Upon Arrival**

506 Upon arrival, confirmation of subject compliance with pre-procedure instructions should be documented
507 on the appropriate case report forms.

508 **3.1.2.3 Preparation for Exam**

509 Subject preparation after arrival and prior to imaging should be standardized among all sites and subjects
510 throughout the conduct of the clinical trial.

- 511 • Measurement and documentation of the subject's weight (and height), though encouraged, is not a
512 requirement of this Profile since the measurand, SUVR, is by definition a ratio of SUVs.
- 513 • The waiting and preparation rooms should be relaxing and warm (> 75° F or 22° C) during the entire
514 uptake period (and for as long as reasonably practicable prior to injection, at least 15 minutes is

suggested as acceptable). Blankets should be provided if necessary. [\(This is for comfort purposes and does not directly impact tracer uptake.\)](#)

- The subject should remain recumbent or may be comfortably seated. [\(This is for comfort purposes and does not directly impact tracer uptake.\)](#)
- After amyloid tracer injection, [\(and if not a full dynamic scan or early frame scan whereby acquisition begins immediately after injection, and if verified with tracer manufacturer's recommendations\)](#) the subject may use the toilet. The subject should void immediately (within 5 – 10 minutes) prior to the PET image acquisition phase of the examination.
- Sedation is not routinely required. It is not certain whether sedation will interfere with amyloid tracer uptake; some preclinical testing indicates a possible interaction, but not all tracers have been tested for possible interaction effects. The decision regarding whether or not to use sedation is beyond the scope of this Profile and requires clinical evaluation of the particular subject for contraindications, as well as knowledge of whether the particular tracer is subject to interaction with the sedating agent. Since these interactions have not been fully defined, subject preparation (with or without sedation) should be consistent across time points for a given subject.
- The amount of fluid intake and use of all medications [for the scan session](#) (e.g., diuretic, sedative) must be documented on the appropriate case report form.
- The subject should remove any bulky items from their pockets such as billfolds, keys, etc. In addition, they should remove eyeglasses, earrings and hair clips/combs (and anything that could cause discomfort while the head is resting in the head holder) if present. They should also remove hearing aids if possible although it is important that they can follow instruction (and hear them if necessary) to remain still while in the scanner.

3.1.3. *Imaging-related Substance Preparation and Administration*

3.1.3.1. Radiotracer Preparation and Administration

3.1.3.1.1 Radiotracer Description and Purpose

The specific amyloid radiotracer being administered should be of high quality and purity. For example, the amyloid seeking radiopharmaceutical must be produced under Current Good Manufacturing Practice as specified by the FDA, EU, European Pharmacopeia or another appropriate national regulatory agency. U.S. regulations such as 21CFR212 or USP<823> Radiopharmaceuticals for Positron Emission Tomography must be followed in the U.S. or for trials submitted to US Regulatory.

While beyond the scope of this document, for any new amyloid tracer it cannot be assumed that SUVR reflects amyloid load without validation, i.e., first full kinetic analysis needs to be performed to check that SUVR has a linear relationship with BP_{ND} .

3.1.3.1.2 Radiotracer Activity Calculation and/or Schedule

The amyloid seeking radiotracer activity administered will depend upon the specific tracer utilized (See Table below). Typically, the dose ranges between about 185 – 370MBq (5 – 10 mCi); for regulatory approved tracers, this should be according to the package insert. [All tracers approved at the time of this Profile have a maximum of 10 ml.](#) The administered activity typically depends upon the local imaging

554 protocol. The local protocol may require fixed activity, or the activity may vary as a function of various
 555 parameters including but not limited to subject size or age or scanning mode. The exact activity and the
 556 time at which activity is calibrated should be recorded. Residual activity remaining in the tubing, syringe or
 557 automated administration system or any activity spilled during injection should be recorded. The objective
 558 is to record the net amount of radiotracer injected into the subject to provide accurate factors for the
 559 calculation of the net SUV.

Parameter	Florbetapir (Amyvid) [1]	Flutemetamol (Vizamyl) [2]	Florbetaben (Neuraceq) [3]
Tracer Admin Activity	370 MBq Max 50 mcg mass dose	185MBq Max 20 mcg mass dose	300 MBq Max 30 mcg mass dose

Formatted Table

Parameter	Entity/Actor	Specification
Administered amyloid Radiotracer Activity	Imaging Technologist, <u>Physician, Nurse, or other qualified Health Professional</u>	<p>The Technologist<u>qualified Health Professional</u> shall</p> <ol style="list-style-type: none"> 1. Assay the pre-injection radiotracer activity (i.e. radioactivity) and time of measurement, 2. Record the time that radiotracer was injected into the subject, 3. Assay the residual activity in the syringe (and readily available tubing and components) after injection and record the time of measurement. 4. Inject the quantity of radiotracer as prescribed in the protocol. <p>These values shall be entered into the scanner during the PET/CT acquisition.</p> <p>For scanners that do not provide for entry of residual activity information, the net injected radioactivity should be manually calculated by decay correcting all measurements to the time of injection and then subtracting the residual radioactivity from the pre-injection radioactivity. The net injected radioactivity is then entered into the scanner during the PET acquisition.</p> <p>All data described herein on activity administration shall be documented.</p>
		All data should be entered into the common data format mechanism (Appendix E).

3.1.3.1.3 Radiotracer Administration Route

Amyloid seeking radiotracer should be administered intravenously through an indwelling catheter (21 gauge or larger) into a large vein (e.g., antecubital vein). This is usually administered as a manual injection; a power injector may be used especially for studies in which SUVR measures of amyloid load are compared with dynamic measures (BP_{ND}). Intravenous ports should not be used, unless no other venous access is available. If a port is used, an additional flush volume should be used. As reproducible and correct administration of radiotracer is required for quantification purposes, extravasation or paravenous administration should be avoided. It should be ensured, for both automated and manual injection, that the radiotracer is not being diluted with saline before or during the injection process. Flushing with saline should only occur after the injection and is recommended when using injection lines.

If an infiltration or extraneous leakage is suspected, the event should be recorded. The anatomical location of the injection site should be documented on the appropriate case report form or in the Common Data Format Mechanism (Appendix E).

Please note that CT contrast agents are not recommended nor supported in the profile.

Parameter	Entity/Actor	Specification
Amyloid radiotracer Administration	Technologist or Physician	<p>Technologist or Physician shall administer the amyloid radiotracer intravenously through an indwelling catheter (24 gauge or larger), preferably into a large vein (e.g., antecubital vein). Intravenous ports should not be used, unless no other venous access is available.</p> <p>A three-way valve system should be attached to the intravenous cannula so as to allow at least a 10 cc normal (0.9% NaCl) saline flush following radiotracer injection.</p>
Suspected infiltration or extraneous leakage	Technologist and/or Physician or Physicist	<p>Technologist shall</p> <ol style="list-style-type: none"> Record the event and expected amount of amyloid tracer: Minor (estimated less than 5%), Moderate (estimated more than 5% and less than 20%), Severe (estimated more than 20%). Estimation will be done based on images and/or known injected volumes. Image the infiltration site.
		Record the event and expected amount of amyloid tracer into the common data format mechanism (Appendix E).

3.2. Image Data Acquisition

This section summarizes the imaging protocols and procedures that shall be performed for an amyloid-PET exam by using either a PET/CT or a dedicated PET scanner with the requirement that a Germanium source can be used to perform attenuation correction. Note that PET scanners that do not measure in some way the attenuation of the brain and use a calculated algorithm for estimating the attenuation and scatter corrections are excluded from this profile. PET/MR scanners are not strictly excluded in this version as long as the repeatability of the SUVRs from these scanners is conformant with the assumptions underlying the Claims. This work was not yet published when this Profile was released. Since the claims of this profile are only valid for the same patient being scanned on the same scanner with the same protocols and analysis, only the repeatability of the PET/MR SUVRs needs to be validated in the context of the Claims, and not the

~~difference in SUVs as compared to PET/CT scanners. In addition, due to their novelty, PET/MR scanners are not covered in this version of the profile. More research and data need to be done with these scanners to understand any differences they may have in quantifying PET amyloid data as compared to PET/CT and dedicated PET scanners.~~ Going forward in this document, PET scanner can mean either a PET/CT or a dedicated PET scanner (or as stated above, PET/MR).

For consistency, clinical trial subjects should be imaged on the same device over the entire course of a study. It is imperative, that the trial sponsor be notified of scanner substitution if it occurs.

For clinical trials with quantitative imaging requirements, a subject should have all scans performed on only one scanner unless quantitative equivalence with a replacement scanner can be clearly demonstrated. However, it should be noted that there are currently no accepted criteria for demonstrating quantitative equivalence between scanners. It is anticipated that future version of this Profile will provide such criteria.

When Amyloid PET imaging is performed across time points for a given subject (longitudinal claim), follow up scans should be performed with identical acquisition parameters as the first (baseline), inclusive of all the parameters required for both the CT and PET acquisitions as described further in this Section.

For amyloid tracer PET/CT perform imaging in the following sequence:

- CT Scout (i.e., topogram or scanogram etc.), followed by the following two acquisitions, in either order (ensuring that the same sequence is performed for a given subject across time points):
- CT (non-contrast) for anatomic localization and attenuation correction and
- PET Emission scan acquisition

For amyloid tracer scan performed on a dedicated PET system (no CT), the first two bulleted steps above are not performed. Instead, perform the Germanium-based attenuation correction scan first and then proceed with the PET Emission scan acquisition.

The issues described in this Section should be addressed in the clinical trial protocol, ideally with consistency across all sites and all subjects (both inter-subject, and intra- and inter-facility) with the target of consistency across all time points (longitudinal utility) for each given subject. The actual details of imaging for each subject at each time point should always be recorded.

3.2.1 Imaging Procedure

The imaging exam consists of two components, the PET emission scan and the transmission scan (performed either with CT or with a Germanium source). From these data sets, the non-attenuation-corrected PET images may be reconstructed for quality control purposes and attenuation-corrected PET images are reconstructed for qualitative interpretation and quantitative analysis. Instrument specifications relevant to the Acquisition Device are included in Section 4.0, Conformance Procedures.

3.2.1.1 Timing of Image Data Acquisition

Amyloid tracer uptake is a dynamic process that may increase at different rates and peak at various times dependent upon multiple variables, different for each radiotracer. Therefore, it is extremely important that (1) in general, the time interval between amyloid tracer administration and the start of emission scan acquisition is consistent and (2) when repeating a scan on the same subject, it is essential to use the same interval between injection and acquisition in scans performed across different time points. The table below lists recommended tracer administration parameters at the time of this Profile for those tracers that have been approved by the FDA in the U.S. However, in all cases, the manufacturer's current labeling

parameters should be consulted, as these may change over time. In addition, while the principles of this profile are fairly generalizable, the specifics apply to the tracers that have already been approved and for which data is available. Note that the durations shown in the table below should be considered minimum durations for image acquisition. For example, for florbetapir, the time window used by ADNI is 20 minutes rather than 10. A full dynamic protocol or longer imaging window (even if not full dynamic) can significantly improve the quality of the data. This will be particularly important for trials in preclinical AD.

Parameter	Florbetapir (Amyvid) [1]	Flutemetamol (Vizamyl) [2]	Florbetaben (Neuraceq) [3]
Tracer Uptake Time (mpi = mins post injection)	30 – 50 mpi	90-60 - 120 - mpi	45 - 130 mpi
Minimum Duration of Imaging Acquisition	10 min	<u>10</u> - 20 min	15 – 20 min

Formatted: Right: -0.14"

Formatted Table

Another amyloid tracer, AV4694, has not yet completed validation in phase III clinical trials and therefore dose and the following acquisition details are preliminary: uptake time 50-70 mpi, and an acquisition duration of 20 minutes.

The “target” tracer uptake time is dependent upon the radiotracer utilized. Reference the above table for acceptable tracer uptake times (in minutes post injection [mpi]) for each of the currently available tracers. The exact time of injection must be recorded; the time of injection initiation should be used as the time to be recorded as the radiotracer injection time. The injection and flush should be completed within one minute with the rate of injection appropriate to the quality of the vein accessed for amyloid tracer administration so as to avoid compromising the integrity of the vein injected.

When performing a follow-up scan on the same subject, especially in the context of therapy response assessment, it is essential to use the same time interval. To minimize variability in longitudinal scanning, for a given subject, the tracer uptake time should be exactly the same at each time point. There is to date no scientific literature quantifying the effect on SUVR with varying tracer uptake times in a no change scenario. The consensus recommendation, to balance practical and ideal, for this Profile is a target window of ± 5 minutes.

If, for scientific reasons, an alternate time (between activity administration and scan acquisition) is specified in a specific protocol, then the rationale for this deviation should be stated; inter-time point consistency must still be followed.

Parameter	Entity/Actor	Specification
Tracer Injection Time	Technologist	The time of amyloid tracer injection shall be entered into PET scanner console during the acquisition.
Tracer Uptake Time:	Technologist	The Technologist shall ensure that the tracer uptake time for the baseline scan is within the acceptable range for the specific radiotracer (see Tracer Uptake Table in Section 3.2.1.1).

Parameter	Entity/Actor	Specification
		When repeating a scan on the same subject, especially in the context of therapy response assessment, the Technologist shall apply the same time interval used at the earlier time point \pm 5 minutes.

654 The following sections describe the imaging procedure.

655 3.2.1.2 Subject Positioning

656 Proper and consistent subject head positioning is critically important for amyloid PET imaging. It is
657 important to take the time necessary to ensure not only that the subject is properly positioned but can
658 comfortably maintain that position throughout the duration of the scanning session. Excessive motion and
659 in particular a difference in the subjects' position between the emission scan and the transmission scan
660 used for attenuation correction is the single most common cause of failed studies.

661 NOTE: The successful implementation of strategies to minimize head motion (and maximize signal to noise)
662 is critical to overall conformance to the Profile requirements. This can be addressed both at the time of
663 image acquisition (through the use of head immobilization techniques described in the paragraphs
664 immediately below) and at the time of image acquisition set-up and reconstruction, described in Section
665 3.3.2.2.1.

666 Position the subjects on the PET or PET-CT scanner table so that their head/~~necks and neck~~ are relaxed.
667 The head should ideally be positioned to have axial slices passing through the cerebellum without
668 intersection with the posterior occipital lobe. This avoids contamination of the posterior cerebellar region
669 by the occipital lobe and the tentorium. To minimize head motion, the subject's head should be
670 immobilized using the institution's head holder/fixation equipment (e.g., thermoplastic mask, tape, etc.). It
671 may be necessary to ~~add~~ place additional pads beneath the neck to provide sufficient support. Vacuum
672 bean bags can also be used in this process. The head should be approximately positioned parallel to the
673 imaginary line between the external canthus of the eye and the external auditory meatus. Lasers are
674 recommended to aid in horizontal and vertical centering. Foam pads can be placed alongside the head for
675 additional support. Velcro straps and/or tape should be used to secure the head position.

676 It should be assured that the head of the subject is positioned in the scanner with the total brain within the
677 field of view (FOV). Special attention must be paid to include the entire cerebellum in the image as this
678 region serves as a reference region for subsequent quantification.

679 For dedicated amyloid tracer PET brain scans, the arms should be positioned down along the body. If the
680 subject is physically unable to maintain arms alongside the body for the entire examination, then the arms
681 can be positioned on their chest or abdomen.

682 Use support devices under the back and/or legs to help decrease the strain on these regions. This will assist
683 in the stabilization of motion in the lower body.

684 The Technologist shall document factors that adversely influence subject positioning or limit the ability to
685 comply with instructions (e.g., remaining motionless).

686

Parameter	Entity/Actor	Specification
Subject	Technologist	The Technologist shall position the subject according to the specific

Parameter	Entity/Actor	Specification
Positioning		protocol specifications consistently for all scans.

Positioning Non-compliance	Technologist	The Technologist shall document issues regarding subject non-compliance with positioning.
		The Technologist shall document issues regarding subject non-compliance with breathing and positioning using the common data format mechanism (Appendix E).

Parameter	Entity/Actor	Specification
Motion non-compliance	Technologist	The Technologist shall document issues regarding subject non-compliance with not remaining still.
		The Technologist shall document issues regarding subject non-compliance (not remaining still) motion using the common data format mechanism (Appendix E).

3.2.1.3 Scanning Coverage and Direction

Anatomic coverage should include from the skull base to the skull vertex, ensuring complete inclusion of the cerebellum. The anatomic coverage should be included in a single bed position.

Parameter	Entity/Actor	Specification
Anatomic Coverage	Technologist	The Technologist shall perform the scan such that the anatomic coverage (including the entire brain from craniocervical junction to vertex) is acquired in a single bed position according to the protocol specifications and the same for all time points.

3.2.1.4 Scanner Acquisition Mode Parameters

We define acquisition mode parameters as those that are specified by the Technologist at the start of the actual PET scan. These include the acquisition time for the single bed position and the acquisition mode (3D mode only). These parameters do not include aspects of the acquisition that occur earlier (e.g., injected amount of 18F-amyloid tracer or uptake duration) or later (e.g., reconstruction parameters) in the overall scan process.

PET Acquisition

If possible, [for SUVR measurement](#) the PET data should be acquired in listmode format (for fullest flexibility

for correcting for head movement) or divided into multiple acquisitions with a maximum of 5 minutes each. If there were no head motion during the scan, a single acquisition frame would be sufficient. However, this is difficult to predict ahead of time, use of multiple time slices is critical for proper motion correction if the subject does not remain still throughout the scan. A full dynamic scan would include additional frames but should also provide for multiple time slices in the late timeframes. Individualized, site-specific acquisition parameters should be determined upon calibration with the appropriate phantom (see below).

Parameter	Entity/Actor	Specification
PET acquisition mode	Study Sponsor	The key 3-D PET acquisition mode parameters (e.g., time per bed position, acquisition mode, etc.) <u>shall be specified</u> in a manner that is expected to produce comparable results regardless of the scanner make and model.
		The key acquisition mode parameters shall be specified according to pre-determined harmonization parameters.
PET acquisition mode	Technologist	The key PET acquisition mode parameters (e.g., time per bed position, acquisition mode, etc.) <u>shall be set as specified</u> by study protocol and used consistently for all patient scans.
		PET should be acquired in listmode format (best) or dynamic time frames of no more than 5 minutes each <u>when possible in order to allow checking and correction for subject motion.</u>

CT Acquisition

For the CT acquisition component of the PET/CT scan, this Profile only addresses the aspects related to the quantitative accuracy of the PET image. In other words, aspects of CT diagnostic accuracy are not addressed in this Profile. In principle, any CT technique (parameters include kVp, mAs, pitch, and collimation) will suffice for accurate corrections for attenuation and scatter. However, it has been shown that for estimating PET tracer uptake in bone, lower kVp CT acquisitions can be more biased. Thus higher kVp (greater than or equal to 80 kVp) CT acquisitions are recommended in general (Abella et al). In addition, if there is the potential for artifacts in the CT image due to the choice of acquisition parameters (e.g., truncation of the CT field of view), then these parameters should be selected appropriately to minimize propagation of artifacts into the PET image through CT-based attenuation and scatter correction.

The actual kVp and exposure (CTDI, DLP) for each subject at each time point should be recorded. CT dose exposure should be appropriately chosen wherever possible, particularly in smaller patients. The radiation principle ALARA (As Low As Reasonably Achievable) for minimizing radiation dose should be considered during imaging protocol development. Refer to educational initiatives, such as Image Wisely (www.imagewisely.org) which provides general information on radiation safety in adult medical imaging, though not specific to amyloid imaging. Note that the ALARA principle is for radiation mitigation and does not address the diagnostic utility of an imaging test.

Parameter	Entity/Actor	Specification
-----------	--------------	---------------

Parameter	Entity/Actor	Specification
CT acquisition mode	Study Sponsor	The key CT acquisition mode parameters (kVp, mAs, pitch, and collimation) shall be specified in a manner that is expected to produce comparable results regardless of the scanner make and model and with the lowest radiation doses consistent for the role of the CT scan: diagnostic CT scan, anatomical localization, or corrections for attenuation and scatter.
		If diagnostic or anatomical localization CT images are not needed, then the CT acquisition mode shall utilize the protocol that delivers the lowest possible amount of radiation dose to the subject (e.g., an ultra-low low dose protocol) that retains the quantitative accuracy of corrections for attenuation and scatter.
CT acquisition mode	Technologist	The key CT acquisition mode parameters (kVp, mAs, pitch, and collimation) shall be set as specified by study protocol and used consistently for all subject scans.
CT acquisition mode	Technologist	If CT kVp is not specified in the study protocol, a minimum kVp of 100 80 shall be used and used consistently for all subject scans.

Parameter	Entity/Actor	Specification
CT Technique: Protocol Design	Technologist / Physician / Medical Physicist	A team comprising a Technologist / Physician / Medical Physicist shall ensure that CT protocols are designed such that dose exposure is the lowest radiation dose necessary to achieve the diagnostic objective. The protocol shall be recorded and documented.
CT Technique: Dose Exposure	Technologist	The Technologist shall ensure that CT dose exposure is the lowest radiation dose necessary to achieve the diagnostic objective.

Regarding CT radiation exposure, the lowest radiation dose necessary to achieve the diagnostic objective should be used. For a given protocol, the purpose of performing the CT scan (i.e., only needed for attenuation correction and/or anatomic localization versus one intended for diagnostic purposes) should be determined. The CT technique (tube current, rotation speed, pitch, collimation, kVp, and slice thickness) used should result in as low as reasonably achievable exposure needed to achieve the necessary PET image quality. The technique used for an imaging session should be repeated for that subject for all subsequent time points assuming it was properly performed on the first study.

3.3. Imaging Data Reconstruction and Post-Processing

740 **3.3.1 Imaging Data Reconstruction**

741 Reconstructed image data is the PET image exactly as produced by the reconstruction process on the PET
 742 scanner, i.e., a PET image volume with no processing other than that occurring during image
 743 reconstruction. This is always a stack of DICOM slices/files constituting a PET image volume that can be
 744 analyzed on one or more of the following: PET scanner console, PET image display workstation, PACS
 745 system, etc. See Section 4.0 for specifications.

746 The PET reconstruction parameters include the choice of reconstruction algorithm, number of iterations
 747 and subsets (for iterative algorithms), the type and amount of smoothing, the field of view, and voxel size.
 748 The quantitative accuracy of the PET image should be independent of the choice of CT reconstruction
 749 parameters, although this has not been uniformly validated. In addition if there is the potential for artifacts
 750 in the CT image due to the choice of processing parameters (e.g., compensation for truncation of the CT
 751 field of view), then these parameters should be selected appropriately to minimize propagation of artifacts
 752 into the PET image through CT-based attenuation and scatter correction. At the time of this profile version,
 753 most scanners have a z-slice thickness less than or equal to 3.27mm, although some older scanners have a
 754 slice thickness of 4.25mm.

Parameter	Entity/Actor	Specification
PET image reconstruction	Study Sponsor	The key PET reconstruction parameters (algorithm, iterations, smoothing, field of view, voxel size) shall be specified in a manner that is expected to produce comparable results regardless of the scanner make and model.
		The key PET image reconstruction parameters shall be specified according to pre-determined harmonization parameters.
PET image reconstruction	Technologist	The key PET reconstruction parameters (algorithm, iterations, smoothing, field of view, voxel size) shall be identical for a given subject across time points.
PET image reconstruction	Technologist	<u>If available, the Point Spread Function (PSF) option can be used; the use or non-use of PSF must be consistent for a given subject across time points. If available, any reconstruction algorithm that uses point spread function (PSF) modeling should NOT be used.</u>
PET image reconstruction	Technologist	If available, the time of flight (TOF) option can be used; the use or non-use of TOF must be consistent for a given subject across time points.
PET Matrix/Voxel size	Technologist	The Technologist shall perform the image reconstruction such that the matrix, slice thickness, and reconstruction zoom shall yield a voxel size of ≤ 2.5 mm in the x and y dimensions and <u>≤ 3.4 mm in the z direction</u> mm in the z dimension. The final size shall not be achieved by re-binning, etc., of the reconstructed images.
Correction	Technologist	All quantitative corrections shall be applied during the image reconstruction process. These include attenuation, scatter,

Parameter	Entity/Actor	Specification
PET image reconstruction	Study Sponsor	The key PET reconstruction parameters (algorithm, iterations, smoothing, field of view, voxel size) shall be specified in a manner that is expected to produce comparable results regardless of the scanner make and model.
		The key PET image reconstruction parameters shall be specified according to pre-determined harmonization parameters.
PET image reconstruction	Technologist	The key PET reconstruction parameters (algorithm, iterations, smoothing, field of view, voxel size) shall be identical for a given subject across time points.
PET image reconstruction	Technologist	If available, the Point Spread Function (PSF) option can be used; the use or non-use of PSF must be consistent for a given subject across time points. If available, any reconstruction algorithm that uses point spread function (PSF) modeling should NOT be used.
PET image reconstruction	Technologist	If available, the time of flight (TOF) option can be used; the use or non-use of TOF must be consistent for a given subject across time points.
factors		random, dead-time, and efficiency normalizations. However, no partial volume correction should be performed.
Calibration factors	Scanner	All necessary calibration factors needed to output PET images in units of Bq/ml shall be automatically applied during the image reconstruction process.

756

757 As part of the image reconstruction and analysis, correction factors for known deviations from the
758 acquisition protocol can potentially be applied. Corrections for known data entry errors and errors in
759 scanner calibration factors should be corrected prior to the generation of the reconstructed images, or
760 immediately afterwards.

761 3.3.2 Image Data Post-processing

762 Processed image data are images that have been transformed in some manner in order to prepare them for
763 additional operations enabling measurement of amyloid burden. Some post-processing operations are
764 typically performed by the PET technologist immediately following the scan. Additional steps may be
765 performed by a core imaging lab, or by an analysis software package accessed by the radiologist or nuclear
766 medicine physician.

767 Initial post-processing operations typically performed by the PET technologist at the imaging site include
768 binning image time frames into a pre-specified discrete frame duration and total number of frames, and
769 putting the images into a spatial orientation specified by the post-processing protocol.

770 In post-processing images, only those steps specified per protocol should be performed, as each transform
771 can slightly modify the image signal, and the intent is to preserve the numerical accuracy of the true PET
772 image values. Studies including full dynamic imaging and kinetic modeling rather than evaluation of a late
773 timeframe static scan may require additional processing as specified in the individual protocol.

3.3.2.1 Ensure image orientation

Whether the image is being prepared for a quantitative “read” by a physician using clinical diagnostic software, or for transmission to a facility for centralized image quality control, processing, and analysis, it is important to ensure that the image is spatially oriented per protocol. This step may occur before or after the creation of a static image below, depending upon the actors and image transfer sequence involved in the protocol.

Parameter	Entity/Actor	Specification
Image orientation	PET technologist	The raw image will be spatially oriented per study protocol.

3.3.2.2 Create Static Image

Depending upon the study protocol, one or more steps may be involved in the creation of the late timeframe static image that is then further processed and used for measurement of the SUVR. In the simplest case, the image may be acquired as a single frame (e.g., 20 minutes long), thus forming a static image without the need to combine timeframes. In this case, Section 3.3.2.2 below is not applicable. Due to the inability to correct for subject motion, this single frame approach may increase the risk of variability outside of the tolerances targeted in this Profile. Alternatively, and commonly in clinical trials, the output may be a set of discrete time frame images (e.g., four five-minute frames) that are then combined into a single static image in subsequent steps. The alternative approach of full dynamic data acquisition typically involves many (>15) frames of variable length, starting with rapid frames acquired immediately at tracer injection.

3.3.2.2.1 Intra-scan inter-timeframe assessment and alignment

For a scan comprised of multiple timeframes, it is important to ensure that the frames are spatially aligned so that the same brain tissue is located in the same coordinates for measurement across the frames. It is preferable that this alignment be performed prior to attenuation correction (that is, as part of the steps in the previous Section 3.3.2.2) in order to prevent embedded error due to misalignment between emission and transmission scan. However, at present, because of limitations in the tools provided with typical scanner workstations, inter-timeframe alignment is typically not performed during image reconstruction and attenuation correction. Rather, visual checks are typically applied and excessive motion may or may not be flagged. If automated, precise tools become available in scanner workstations in the future, the inter-frame alignment and static image formation described in this section may become part of the image reconstruction process. Even when inter-timeframe alignment is performed prior to attenuation correction or at the imaging site, it is important that the discrete binned frames prior to inter-frame alignment, the transmission scan, and the alignment parameters applied, be made available for quality control in later processing and analysis steps.

Inter-frame alignment is typically performed using automated software that employs mathematical fitting algorithms to match the image from each timeframe to a reference. The reference frame may be that acquired closest to the time of transmission scan (e.g., the first frame in late frame acquisition if the transmission scan precedes the emission scan) or as otherwise stated per protocol. The amounts of

812 translation or linear adjustment, in each of the x, y, and z directions, and the amount of rotational
 813 adjustment in each of three orthogonal directions are measured by the software. Depending upon the
 814 software platform, these parameters are available for review by the image analyst, or may be pre-
 815 programmed to make pass/fail or other decisions. Large values (greater than 4 degree rotation or 4 mm
 816 translation) indicate that subject motion is likely embedded within one or more frames introducing noise
 817 (signal variability) that cannot be removed from those particular frames. In addition, unless attenuation
 818 correction was performed on a frame by frame basis during image reconstruction, large values indicate that
 819 emission-transmission scan misalignment error is also embedded in one or more frames.

820 The study protocol should define the allowable translation and rotation permitted between the reference
 821 frames and other frames. Frames exceeding these limits may be removed, with the following caveats: (a)
 822 removal of too many frames (e.g. more than half of the total acquisition window) may result in inadequate
 823 total counts and a noisy scan; and (b) frame removal should be consistent across longitudinal scans for the
 824 same subject, or slight error can be introduced. Note that particularly in certain subject populations it is not
 825 uncommon to observe translational or rotational motion exceeding 2 mm or 2 degrees, and exceeding 5
 826 mm or 5 degrees in some scans. Typical clinical studies of MCI and AD patients have had mean (standard
 827 deviation) values of 1.7 (1.1) mm for maximum translation and 1.5 (1.1) degrees for maximum rotation.
 828 Motion tends to worsen with longer duration scans. The decision to extend allowable motion thresholds
 829 becomes a balance between retaining subject frames and tolerating increased signal variability.

830 Currently, most scanner workstations do not provide readily used automated tools for inter-frame motion
 831 measurement and correction, and automated alignment to the transmission (or CT) scan prior to
 832 attenuation correction. Once such tools are available, the activity of frame alignment would best be
 833 performed prior to attenuation correction, to prevent embedded attenuation correction error that cannot
 834 be removed through subsequent inter-frame alignment. On occasion, even with current tools, this can be
 835 performed at the site. Even when realignment at the imaging site becomes feasible, the inter-frame
 836 alignment parameters of the original scan acquisition should be available to the Image Analyst, as under
 837 certain conditions enough within-frame motion may have occurred to merit removal of the frame
 838 regardless of inter-frame correction.

839

Parameter	Entity/Actor	Specification
Inter timeframe consistency	Image analyst or, pending protocol, PET technologist	When a multi-frame PET scan is provided, the translational and rotational adjustment required to align the frames will be assessed prior to combining frames into a single scan.
Action based on inter-timeframe consistency check	Image analyst or, pending protocol, PET technologist	If <u>inter-frame alignment has been performed</u> prior to attenuation correction, frames will be removed if inter-frame translation exceeds a recommended threshold of 4 mm or inter-frame rotation exceeds 4 degrees (or less if indicated by study protocol) or <u>if inter-frame alignment has not been performed</u> prior to attenuation correction, frames will be removed if inter-frame translation exceeds a recommended threshold of 4 mm or inter-frame rotation exceeds a recommended threshold of 4 degrees from position of the CT scan used for attenuation correction (or less if indicated by study

Formatted Table

Parameter	Entity/Actor	Specification
		protocol).

Formatted Table

840

841 **3.3.2.2 Combine discrete timeframes**

842 Once all or a subpopulation of the appropriately aligned timeframes have been identified, a composite
 843 image is generated for further processing and analysis. For late timeframe scans, this is accomplished
 844 through averaging or summation of the timeframes into a single image volume. In full dynamic scanning, a
 845 “parametric” image can be created through a more complex procedure that involves measuring signal in
 846 amyloid “rich” (having high tracer binding) and amyloid “poor” (low tracer binding) regions, or using blood
 847 measurements if available, and solving simultaneous equations to determine voxel values. The parametric
 848 image can then be measured using the same Volume of Interest or other methods described below, with
 849 the difference that the measure becomes a Distribution Volume Ratio (DVR) rather than SUVR.

850

<u>Parameter</u>	<u>Entity/Actor</u>	<u>Specification</u>
Static Image generation	Image analyst or image processing workstation	Only timeframes identified as appropriately aligned will be included in this image generation.

851

852 **3.3.3 Imaging Data Storage and Transfer**

853 Discussions of archiving PET data often mention 'raw data'. This is an ambiguous term as it can refer to:
 854 **scanner raw data** (i.e., sinograms or list-mode) or image raw data. To avoid confusion, the term raw data
 855 should not be used without making it clear which form is under discussion.

Formatted: Justified

856 **Image raw data** is the image data exactly as produced by the reconstruction process on the PET or PET/CT
 857 scanner. i.e., a stack of DICOM slices/files constituting a PET image volume with no processing other than
 858 that occurring during image reconstruction. This is typically a stack of DICOM slices/files constituting a PET
 859 image volume that can be analyzed on one or more of the following: PET scanner console, PET image
 860 display workstation, PACS system, etc. If inter-frame alignment is performed prior to attenuation
 861 correction, then “raw data” may include both the emission and transmission frames prior to any inter-
 862 frame or inter-scan alignment, the realigned frames that were used for attenuation correction, and the
 863 attenuation corrected frames.

864 **Post-processed image data** are images that have been transformed after reconstruction in some manner.
 865 This is typically a stack of DICOM slices/files constituting a PET image volume that can still be analyzed on
 866 one or more of the following: PET scanner console, PET image display workstation, PACS system, etc.

867 For archiving at the local site or imaging core lab (if relevant), the most important data are the original
 868 images, i.e. the image raw data. In the unlikely event that the scanner raw data (which should be archived
 869 by the local site) is required for later reprocessing; this should be made clear in the protocol.

870

Parameter	Entity/Actor	Specification
-----------	--------------	---------------

Parameter	Entity/Actor	Specification
Data archiving: raw images	Technologist	The originally reconstructed PET images (image raw data), with attenuation correction, and CT images shall always be archived at the local site. If scanner raw data need to be archived for future reprocessing, this should be defined prospectively in the Protocol.
Data archiving: post-processed images	Image analyst	If a static image has been generated by aligning frames and summing or averaging discrete timeframes, or through other parametric image generation, the image will be archived at the site where the static image generation occurred.

871

872 **3.4. Image Analysis**

873 The Image Analyst, through interaction with the Workstation Analysis tools, shall be able to perform
874 specified measurements [and analyses](#) on the images. Image Analysis has qualitative and quantitative tasks.
875 Both tasks require high quality image submission and consistency of image interpretation. Quantitative
876 imaging requires additional system characteristics described further in Section 3.2, Image Data Acquisition,
877 and Section 3.6, Quality Control, of this Profile.

878 **3.4.1 Input Data**

879 The output of image Reconstruction and Post-processing (inclusive of Static Image Generation) resulting in
880 a single image volume, corrected for attenuation, scatter, randoms and radiotracer decay, is considered the
881 input for static scan Image Analysis. In the case of full dynamic imaging for kinetic analysis, the Post-
882 processing output may be a set of timeframes. The original input data- [\(deidentified when applicable\)](#)
883 [received](#), without modification, should be maintained as a separate file (or set of files), to be stored along
884 with the processed data that is ultimately used to perform measurements. (See Section 3.2).

885 **3.4.2 Image Quality Control and Preparation**

886 Before Image Analysis is performed, stringent image quality control is essential to ensure that images are
887 suitable for processing and analysis. The elements of raw image quality control that should be performed
888 during performance of post-reconstruction processing are defined in Section 3.3, Image Post-Processing.
889 Elements of post-processed image quality control that should be performed by the Image Analyst or the
890 Processing Workstation software prior to further processing and analysis of the image data are listed in
891 Section 3.6, Quality Control.

892

893 **3.4.2.1 Correction for Partial Volume Effects (PVE)**

894 Partial Volume Effects Correction (PVEc) is ~~NOT~~ recommended as a “by default” step in this Profile due
895 to the fact that the process itself can introduce a great deal of variability, countering the tolerance goals of
896 the Profile. However, we discuss this step here, as it may be included in certain study protocols particularly
897 if methodology is systematically employed that does not increase variability. As background on this topic,

Formatted: Justified

Formatted: Justified

898 due to the limits of PET scanner resolution, the signal measured at the borders of white and gray tissue, or
 899 tissue and cerebrospinal fluid (CSF) can contain contributions from both types of tissue within the
 900 boundaries of the same voxel. In particular, some amyloid PET tracers have high levels of nonspecific white
 901 matter uptake, producing high signal intensity that “spills into” neighboring gray tissue measures. In
 902 addition, neurodegenerative patients may exhibit substantial, progressive atrophy, increasing spill-in from
 903 CSF that can dilute increases or accentuate decreases originating from the atrophic tissue elements.
 904 Several different mathematical algorithms and approaches have been developed to correct or compensate
 905 for PVE and tissue atrophy. However, these approaches are not necessarily sensible in the setting of
 906 amyloid imaging and quantification. Simply applying correction for the loss of cerebral gray matter results
 907 in upscaling of image signal intensity, and is most appropriate when the tissue origin of the signal is lost,
 908 resulting in the atrophy (~~ex-such as~~ loss of synaptic neuropil in [\[18F\]2-fluoro-D-2-deoxyglucose \(FDG\)](#)
 909 cerebral glucose metabolism imaging). In the case of amyloid ~~deposits-deposition~~ in neurodegenerative
 910 dementia, however, the deposits are not contained with normal cerebral gray matter elements; ~~a. Amyloid~~
 911 plaques are extracellular accumulations and are unlikely to degenerate as gray matter atrophies due to
 912 losses of synapses and neurons ensues. Thus, applying gray matter atrophy-correction PVEc may
 913 inappropriately “upscale” the amyloid signal from atrophic cortical regions. Usual PVEc approaches result
 914 in a new image, typically containing only gray matter, and has been shown to increase the apparent
 915 amyloid in AD patients by as much as 30% to 56%. The most sensible approach to PVEc in amyloid images is
 916 to apply correction for spillover from subcortical white matter into the gray matter regions, which is likely
 917 to become increasingly problematic as the cortical gray matter becomes atrophic. Appropriate use of PVEc
 918 can potentially help to increase sensitivity to longitudinal change, and to reduce error associated with
 919 changes in atrophy or white matter uptake. However, PVEc methods can also introduce variability, and
 920 results are highly sensitive to subjective selections of the parameters used in calculating the correction.
 921 Effects upon measurement of longitudinal change have varied from no effect to an increase in measured
 922 change. The tradeoff between benefit vs. these considerations must be considered and the decision as to
 923 whether or not to use may be study dependent. The point in the process at which PVEc ~~-correction- is~~
 924 applied may vary, for example either applied to spatially normalized images or to native images, prior to or
 925 after the creation of a SUVR image.

926 **3.4.2.2 Image Smoothing**

927 Depending upon whether more than one scanner and reconstruction software combination is being used to
 928 acquire patient data, and the objective of the image analysis, it may be necessary to smooth the image.
 929 Smoothing applies a mathematical filter to the image signal at each voxel to help compensate for
 930 differences in spatial resolution that exist between different scanners. Even if the same scanner is used for
 931 each visit by a particular subject, being able to compare the SUVR value to a threshold derived using images
 932 from multiple scanners, or to other study subjects whose data is collected on other scanners, requires
 933 adjustment for scanner differences. If not reconciled, these differences can cause a few percent difference
 934 in SUVR ([Joshi et al, 2009](#)).

935 By “spreading” signal out, smoothing also helps to increase the spatial overlap of amyloid accumulation
 936 across different subjects, increasing the ability to identify group effects in voxel-based comparisons.
 937 However, smoothing also dilutes signal, particularly in small structures, and can also increase the mixing of
 938 white, gray, and CSF signal.

Commented [DM1]: Joshi A, Koeppe RA, Fessler JA. Reducing between scanner differences in multi-center PET studies. Neuroimage. 2009 May 15;46(1):154-9.

Parameter	Entity/Actor	Specification
-----------	--------------	---------------

Image smoothing	Image analyst	When combining scans from different scanners and/or reconstruction software that produce different image resolutions, filtering will be applied per protocol to produce comparable signal for the same amount of radioactivity.
-----------------	---------------	---

940

941 **3.4.3 Methods to Be Used**

942 The methodology and sequence of tasks used to perform amyloid tracer analysis have historically varied
 943 across studies depending upon the radiotracer, image analysis workstation, software workflow and
 944 parameters determined to be of interest in the study design. Processing and analysis steps have ranged
 945 from a manual workflow to a semiautomatic workflow (which requires some user interaction with the
 946 workstation) to an automatic workflow (with little or no user interaction), with various alternatives possible
 947 at each step. An outline of the major steps typically included in the workflow is provided below. These
 948 steps are associated with a Standardized Uptake Value Ratio (SUVR) calculation approach using an
 949 equilibrium stage “late timeframe” image. Details, considerations impacting analysis reliability, and
 950 guidelines are then provided. Points where order of operations can vary without impacting end result, such
 951 as the option to generate an SUVR image prior to target region measurement, are noted. Notes are also
 952 included regarding the alternative use of the full dynamic scan and kinetic modeling to produce measures
 953 of amyloid burden.

Spatially match subject scan with source image for ROI definition



(optional) Create SUVR image



Measure regions of interest and calculate SUVRs

Spatially match subject scan with source image on which regions of interest (ROIs) have been defined. This may be the subject’s MRI scan, segmented into anatomical regions, or it may be a “template” MRI or PET scan on which regions have been pre-defined. If a template is used, a spatial transformation or “warping” is required to match the template and subject scan so that the defined regions can be mapped onto the subject scan.


As an optional step, create an intensity-normalized version of the scan (“Standardized Uptake Value Ratio”, or “SUVR” image) by dividing all voxels in the scan by the average measured intensity in a selected reference region (such as cerebellum). This can be useful for visual assessment and comparisons between scans.

Apply boundaries (“masks”) for target regions of interest and measure average intensity. If the image has already been intensity normalized to the selected reference region, these are equal to the SUVR. If the image has not been intensity normalized, or to use a different reference region, measure reference region intensity and calculate SUVR as target region intensity divided by reference region intensity. Other voxel-based analyses may also be performed.

Formatted: Centered

954

955



956

957

958 Figure 4. Typical steps in image processing and measurement for SUVR calculation

959

960 Despite variability in workflows that may be applied, several fundamental factors can impact the accuracy
961 and reproducibility of measurement. These [factors](#) are discussed below and guidance [is](#) provided to achieve
962 accuracy and reproducibility.

963 **3.4.3.1 Spatially Match Subject and Template**

964 The fitting of Volumes of Interest (VOIs) to a scan for amyloid studies has typically been performed by

965 automated software, reducing the subjectivity, inter-reader differences, and labor intensity of manual
 966 delineation. In order to measure pre-defined VOIs for SUVR calculation (or DVR in the case of full dynamic
 967 scanning), it is necessary to map these spatial boundaries to the subject's specific brain morphology or vice
 968 versa. ~~The following approaches can be applied: (a) Spatial mapping of individual brain scans to a template
 969 brain having pre-defined VOI boundaries; (b) Spatial mapping of the template brain and pre-defined VOI
 970 boundaries based upon a probabilistic atlas of gray matter segments or otherwise delineated regions to the
 971 individual brain scans; and (c) Use of segmentation algorithms that "find" each anatomical structure of
 972 interest within the subject's native morphology using the subject's MRI (e.g., Freesurfer). Mapping
 973 individual subject scans to a brain template is also required to allow scans to be compared to one another
 974 using voxel-based analysis. Segmentation results are dependent upon the MRI sequence used; even the
 975 same sequence may produce different results on different MRI scanners.~~

978 3.4.3.1.1 "Fuse" MRI and PET images

979 The majority of amyloid test-retest studies and most clinical trials with quantitative amyloid imaging have
 980 used the subject's MRI scan as a high resolution vehicle for the spatial mapping approaches described
 981 above. With clinical application as a consideration, processing pipelines using specific amyloid PET
 982 radiotracers have been developed to use PET-to-PET spatial transformation. An optimized PET-to-PET
 983 transformation approach has been developed for flutemetamol, and similar approaches have been
 984 developed for other tracers. In cases where an MRI is used, the subject's MRI and PET are "fused" or co-
 985 registered to one another using a linear transformation performed by automated software. While either
 986 MRI or PET can serve as the target to which the other is co-registered, registering the MRI to the PET
 987 prevents interpolation of the PET image. However, preserving the resolution of the MRI image, typically
 988 higher than that of the original PET, is useful for later operations including segmentation of the MRI and
 989 transformation to template space. This can be accomplished by co-registering the PET to MRI, or by up-
 990 sampling the PET prior to co-registration of the MRI to the PET or otherwise preserving output resolution.

991 Since mapping operations performed on the MRI will be applied to its co-registered PET scan, it is critical to
 992 ensure that the PET and MRI have been properly aligned to one another. Visual inspection should be
 993 conducted with careful attention to proper left-right orientation and alignment in all three planes
 994 (transaxial, sagittal, and coronal); quantitative goodness of fit measures can also be applied. Successful
 995 fusion may be indirectly checked through verification of correct VOI placement and/or correct spatial
 996 normalization. However, if misalignment occurs, one must backtrack to determine where in the process
 997 this happened, and verification of each step is recommended. Automated methods to assure goodness of
 998 fit may also be employed.

Parameter	Entity/Actor	Specification
PET and MRI image fusion	Image analyst	When coregistering a subject's PET and MRI images, accurate alignment of the images in all planes (transaxial, coronal, sagittal) will be verified.

3.4.3.1.2 Longitudinal PET co-registration

For longitudinal amyloid measurement, co-registering subsequent PET scans to the baseline PET scan is recommended, as separate MRI to PET co-registrations or separate spatial warping operations (described below) may produce slightly different alignments. This can cause differences in VOI measurement, and even a few percent can be significant for longitudinal evaluation. Goodness of fit of inter-PET scan alignment should be visually verified; quantitative metrics such as correlation can also be applied.

Successful longitudinal co-registration may again be indirectly checked through verification of correct VOI placement and/or correct spatial normalization. In addition, if a process involving separate spatial normalization of longitudinal scans is applied and achieves comparable fit, the result would be acceptable. However, if misalignment occurs, one must backtrack to determine where in the process this happened, and therefore explicit verification of proper longitudinal coregistration is recommended.

It is noted here that some studies (unpublished, multiple groups) have shown that a superior longitudinal alignment of sequential PET scans can be achieved when co-registering the series of PET scans together rather than separately co-registering each PET to the MRI. However, it is also noted that in cases of substantial longitudinal atrophy or ventricular expansion, care must be taken in ensuring that the VOIs applied to each scan account for the actual gray tissue present in the brain.

In addition, it is also noted that although not ordinarily expected, it is possible for longitudinal structural changes (abnormalities) to occur that impact the ability to use a common mapping across scans. One such example is cerebellar encephalomalacia. However, such an event is not within the scope of this profile version and it is rather recommended to exclude the subject in this case or to use target and reference regions that are unaffected by the abnormality.

Parameter	Entity/Actor	Specification
Co-registration of longitudinal scans	Image analyst	When coregistering a subject’s longitudinal PET images, accurate alignment of the images in all directions (transaxial, coronal, sagittal) will be verified.

3.4.3.1.3 Spatial Mapping of Subject Image and Template Image

The following approaches can be applied for spatial mapping:

(a) Spatial mapping (“warping”) of individual brain scans to a template brain having pre-defined VOI boundaries. The VOIs are then measured in “template space”, with some spatial distortion to the original brain tissue. The goodness of fit of subject to template depends upon multiple factors including: the spatial warping algorithm applied, the parameters selected for the warping algorithm, and the template selected. For example, scans acquired in an aging, atrophic population may warp in a superior manner to a template that was also derived from an aging, atrophic population.

(b) Spatial mapping of the template brain and pre-defined VOI boundaries to the individual brain scans. In this case, the VOIs are still probabilistic but are mapped to the subject’s original morphology.

(c) Use of segmentation algorithms that identify each anatomical structure of interest within the subject’s native morphology using the subject’s MRI (e.g., Freesurfer). The resulting segmentation (i.e. the

1036 identification of various gray tissue regions) can vary depending upon several factors including: the
 1037 segmentation software and version applied, the operating system on which the software is run, the
 1038 parameters selected in the segmentation software, the MRI sequence used, and .

1039 Depending upon the approach taken to map regions of interest or reference regions to the PET scan, spatial
 1040 transformation (or “warping”) between the image and a template image may be necessary. If the subject’s
 1041 native space MRI is segmented and used to define region of interest boundaries, and no voxel-based group
 1042 analyses are performed, then spatial warping is not required. However, if regions pre-defined in template
 1043 space are to be applied to the scan, then the transformation is a critical step.

1044 The mapping between subject image and template image is accomplished through automated spatial
 1045 normalization or warping software algorithms. When an MRI is used, the transformation is determined
 1046 though a “warp” between subject MRI and template, and the same mathematical transform is applied to
 1047 the coregistered PET scan (if transforming to template space) and/or to the ROIs (if transforming to the
 1048 native subject scan). The accuracy of the spatial transformation depends upon the algorithm. Certain
 1049 software and software versions have shown superior alignment of cerebellum, deep structures such as
 1050 putamen and medial temporal regions, and ventricles as compared to older algorithms (Klein et al, 2009).
 1051 In addition, the template to which images are warped can impact goodness of fit and optimization for the
 1052 study population may be of use.

1053 When an MRI is not available, the subject PET scan can be transformed directly to the template PET. Since
 1054 the signal within gray matter and the intensity contrast between gray and white matter in a negative
 1055 amyloid scan are substantially different than those in an amyloid positive scan, images at the extremes of
 1056 positive and negative may not spatially normalize well. To address this, various approaches have been
 1057 developed that test the fit to a series of templates (Lundqvist et al, 2013), selecting the best fit. Other
 1058 confounds in PET-based spatial normalization can occur when the amyloid PET image has high intensity
 1059 signal in portions of dura or skull, or missing (truncated) tissue at the top or bottom of the brain. Various
 1060 additional steps have been employed to address these issues.

1061 Regardless of the approach used for spatial normalization, an accurate match between subject and
 1062 template is critical to amyloid measurement. Goodness of fit should be evaluated using visual inspection,
 1063 and quantitative goodness of fit algorithms can also be applied. As a note, ad hoc manual (e.g. touch
 1064 screen or mouse based) modification of warping results should not be used as changing the fit for one set
 1065 of slices through “eyeballing” is very likely to introduce error into other slices.

Parameter	Entity/Actor	Specification
Spatial mapping with template image	Image analyst	When spatially mapping a subject image and a template image to one another accurate alignment of the images in all directions (transaxial, coronal, sagittal) will be verified visually.

Formatted: Left

1068 **3.4.3.2 VOI Placement: Target / Reference**

1069 **3.4.3.2.1 Determine Target Regions for Measurement**

1070 The selection and delineation of target regions for amyloid measurement vary depending upon study

objectives and should be specified in the protocol. For clinical application, some manufacturers have specified predefined VOIs associated with a threshold SUVR that they have correlated to autopsy data. Some clinical trials have used a cortical average consisting of 4 – 6 regions, with individual regional amyloid measures providing further information. When “emerging” subjects with amyloid levels nearer to threshold are studied in clinical trials, analysis of specific sub-regions may become important.

Given a specified anatomical region (e.g., frontal, or cingulate), there are several ways to define the tissue that is included in the region, and several considerations that are not mutually exclusive, listed below. Automation of region definition is important given the high level of subjectivity that can be associated with manual definition.

- *Region Boundaries*: Some approaches use the entire anatomical region, whereas others define a sub-region empirically determined to accumulate greatest amyloid burden.
- *Method to match the region to subject’s anatomy*: Some methods apply a standard atlas of region definitions (pre-defined anatomical boundaries based upon reference brains), and rely upon the transformation between the subject’s morphology and the atlas template to match the atlas regions to the subject. These may be referred to as “probabilistic” regions. Other approaches estimate anatomical boundaries based upon the individual subject’s MRI, incorporating atlas reference information in a more complex way (e.g., Freesurfer).
- *Region confinement to gray tissue*: When atlas based regions are applied, these may or may not be thresholded (restricted) using the gray tissue segment from the subject’s MRI. This masking can help to assure alignment between template regions and the subject’s actual morphology, and can be done using either native space images or warped images.
- *Region erosion from surrounding tissue or CSF*: VOI boundaries may be eroded (e.g., perimeter reduced by one to two voxels) away from the neighboring CSF and white tissues, in order to reduce atrophy effects and spillover from non-gray tissue types. This is most often applied to probabilistic regions that tend to be larger and incorporate tissue adjacent to gray matter.
- *“Native space” vs. “Template space”*: VOIs may be defined only in template space, for measuring the subject’s warped scan, or may be transformed to the subject’s native scan. Use of the native scan can reduce interpolation and signal changes arising from stretching or compressing subject anatomy.

Comparisons of different approaches to regional definition, including whether native vs. template scans are used, have yielded high correlation coefficients (Landau et al, 2013). However, it is important to note that measurement of different portions of tissue will give different results. It is therefore important that the same tissue definition be applied across scans and across subjects within a study.

Parameter	Entity/Actor	Specification
Target Region Definition	Image Analyst	The same target region definitions (which may be transformed to each individual subject’s morphology) will be applied consistently to subjects and across a study.

3.4.3.2.2 Determine Reference Region

The definition of the reference region is one of the most critical aspects of image analysis. Reference regions are used for image comparison because raw image counts for the same subject will change from scan to scan due to injected dose, scanner calibration, or other factors unrelated to amyloid. If every region in the brain changes in the same proportion due to these factors, then such changes will cancel by taking the ratio of target region to reference region. The reference region is typically a region that does not accumulate or lose amyloid, enabling changes in target regions due to amyloid to be detected.

This Profile does not dictate a particular reference region, since tracer manufacturers and leading research institutions have differed and continue to evolve, on this topic. However, there is a growing body of evidence that certain reference regions exhibit less longitudinal variability and it has been shown that the optimal reference region can be different for each radiotracer (Villemagne, AAIC 2015). In addition, certain practices should be followed to minimize variability arising from the scanner and to ensure the validity of the reference measurement. These considerations are discussed below.

The cerebellar cortex (gray matter) has been a reference region of choice in numerous studies of amyloid since it typically does not accumulate fibrillar amyloid and because its gray tissue kinetics are assumed be reasonably matched to those of gray tissue target regions. Because of its low signal and lack of binding, the cerebellar cortex provides the most sensitive reference for measuring cross sectional differences. However, due to its low signal level, small swings in value will create large swings in calculated SUVR. Further, the physical location of the cerebellum toward the edge of the scanner transaxial field of view makes it susceptible to edge noise, scatter, and tissue exclusion (particularly in scanners with a shorter axial field of view). In head rotation and in emission-transmission scan misalignment, the posterior edge of the cerebellar cortex can be particularly impacted. In addition, slight shifts in position can cause a blending of white and gray tissue that will impact the reference measurement. Further, the cerebellum is located in transaxial slices that are not in proximity to several typical target VOIs, and signal in those slices may not change in the same way due to technical factors. In longitudinal studies, for one radiotracer, the cerebellar cortex has been demonstrated to show stability over time (Villemagne, AAIC 2015) while for others variability with regard to measured change has been shown, decreasing statistical power. Even in cross-sectional measurements, technical noise embedded in the cerebellum (or any reference region) may cause a subject whose amyloid burden is at the threshold of positivity to “tip” in one direction or another. If the reference regions does include the cerebellum, it is recommended to omit the superior portions of the cerebellum to avoid radiotracer contamination form surrounding structures such as the occipital cortex or the fusiform gyrus and to omit the lowest slices that exhibit greatest variability. These strategies have been employed in various studies (Shcherbinin et al, 2016; Barrtet et al, 2016; Pontecorvo et al, 2017; Hahn et al, 2017). At a minimum, the inferior margin of the cerebellar reference boundaries should not extend to the edge of the FOV, where the greatest technical variability occurs. Alternate reference region comparisons are also recommended to ensure that noise has not driven the SUVR result.

Use of whole cerebellum has been specified as a reference of choice with some ~~ligands~~ PET tracers (such as florbetapir), and can reduce variability arising from shifts that include more white matter (Joshi, JNM 2015), since ~~#-white matter~~ is already included. However, the same issues with spatial location, edge noise, and lower average signal still apply. As an alternative reference, the pons has been applied in multiple studies, and found to have a slightly lower variability. Its advantages include higher signal due to white matter inclusion, and more central location in the brain at a slightly further distance from the edge of the scanner transaxial field of view. Some studies using florbetapir, flutemetamol and 11C-PIB have found that the pons exhibited lower longitudinal variability than a cerebellar reference region (Thurfjell et al, 2014; Shokouhi et

Commented [DM2]: Shcherbinin S, Schwarz AJ, Joshi A, Navitsky M, Flitter M, Shankle WR, Devous MD Sr, Mintun MA. Kinetics of the Tau PET Tracer 18F-AV-1451 (T807) in Subjects with Normal Cognitive Function, Mild Cognitive Impairment, and Alzheimer Disease. J Nucl Med. 2016 Oct;57(10):1535-1542. Epub 2016 May 5. PubMed PMID: 27151986. 'The AAL-based cerebellum crus region was modified by translating it by 6 mm in the z-axis to avoid overlap with noncerebellar space. The resulting regions are shown in Figure 1.'

Barret O, Alagille D, Sanabria S, Comley RA, Weimer RM, Borroni E, Mintun M, Seneca N, Papin C, Morley T, Marek K, Seibyl JP, Tamagnan GD, Jennings D. Kinetic Modeling of the Tau PET Tracer 18F-AV-1451 in Human Healthy Volunteers and Alzheimer's Disease Subjects. J Nucl Med. 2016 Dec 1. pii: jnumed.116.182881. [Epub ahead of print] PubMed PMID: 27908967.

'The cerebellar cortex region was eroded away from other regions by 8 mm to minimize spill-over, in particular from the temporal and occipital regions.'

Pontecorvo MJ, Devous MD Sr, Navitsky M, Lu M, Salloway S, Schaeff FW, Jennings D, Arora AK, McGeehan A, Lim NC, Xiong H, Joshi AD, Siderowf A, Mintun MA; 18F-AV-1451-A05 investigators.. Relationships between flortaucipir PET tau binding and amyloid burden, clinical diagnosis, age and cognition. Brain. 2017 Mar 1;140(3):748-763. doi: 10.1093/brain/aww334. PubMed PMID: 28077397; PubMed Central PMCID: PMC5382945. 'A cerebellar grey matter region derived from the cerebellar crustaneous (cerecr-1 region of interest from AAL) modified by translating it inferiorly by 6 mm was chosen.'

Hahn A, Schain M, Erlandsson M, Sjolín P, James GM, Strandberg OT, Hagerstrom D, Lanzenberger R, Jogi J, Olsson TG, Smith R, Hansson O. Modeling Strategies for Quantification of In Vivo (18)F-AV-1451 Binding in Patients with Tau Pathology. J Nucl Med. 2017 Apr;58(4):623-631. doi: 10.2967/jnumed.116.174508. Epub 2016 Oct 20. PubMed PMID: 27765859.

Commented [DM3]: Thurfjell et al, Automated Quantification of 18F-Flutemetamol PET Activity for Categorizing Scans as Negative or Positive for Brain Amyloid: Concordance with Visual Image Reads. J Nucl Med October 1, 2014 vol. 55 no. 10 1623-1628. doi: G610.2967/jnumed.114.142109

1152 al, 2016; Edison et al, 2012). However, the narrow cylindrical size and shape of the pons
 1153 make it vulnerable to subject motion, and it, too, can be affected by technical variability. Subcortical white
 1154 matter provides another alternate reference region, with the advantages of higher signal, larger
 1155 measurement volume, transaxial alignment with target regions of interest. Studies have demonstrated
 1156 benefit in lower variability using subcortical white matter, and thus greater statistical power in measuring
 1157 longitudinal change, relative to other reference regions (Reference needed Chen et al, 2015; Brendel et al,
 1158 2015; Schwarz et al, 2016; Blautzik et al, 2017). One consideration in the use of a white matter reference is
 1159 that the kinetic properties of white matter differ from those of the gray tissue target regions, with unclear
 1160 impact upon measurement validity. There is not yet a published full dynamic modeling study of white
 1161 matter as a reference. White matter axonal integrity may decline with AD progression and age, potentially
 1162 increasing advantageous cross sectional differences between AD and Normal, and introducing possible
 1163 variability over time. However, findings seem to support the ability to detect increases in amyloid positive
 1164 populations as expected and seen with gray tissue reference regions, yet with lower variability (ideally this
 1165 would be compared to full kinetic modeling results to demonstrate accuracy). When white matter is used,
 1166 careful definition based upon the MRI, with erosion from neighboring gray tissue, is recommended.
 1167 Combinations of whole cerebellum, pons, and subcortical white matter, or cerebellar white matter and
 1168 pons, or "amyloid poor" gray regions other than cerebellum have also been applied with reductions in
 1169 longitudinal variability (for florbetapir) resulting in increased statistical power (add a reference to justify the
 1170 composite reference region Tryputsen et al, 2015; Landau et al, 2015). It should be noted, however, that
 1171 the signal from reference regions using subcortical white matter may be affected by vascular pathology,
 1172 common in the elderly. It is finally noted that regions comprised of both gray and white matter, whether
 1173 whole cerebellum or composite regions, may include divergent changes over time. These may be a suitable
 1174 match for probabilistic target regions that include both gray and white matter, or given white matter
 1175 spillover into gray tissue. However, for "pure" gray target regions, their longitudinal use may introduce
 1176 some non-amyloid related variability. All of this must be weighed against other sources of variability arising
 1177 from use of a pure cerebellar cortex reference due to low signal, scatter, subject motion, and differences in
 1178 the axial placement from scan to scan.
 1179 "Amyloid poor" gray tissue in the same axial plane as the target regions can provide the dual benefit of co-
 1180 location, protecting against sometimes major changes arising from differences in slice sensitivity in a
 1181 scanner, as well as matching of gray tissue perfusion rates. A caveat is that if these regions slowly
 1182 accumulate amyloid or do have amyloid accumulation that can be removed during an anti-amyloid drug
 1183 study, reference stability may be compromised.
 1184 The With the above caveats in mind, the use of a combined reference, subcortical white matter, or other
 1185 stable "amyloid poor" regions proximal to target regions may be advised, depending on the
 1186 radiotracer (radiotracer dependent), particularly for longitudinal studies and for measurement of amyloid
 1187 in subjects near the threshold of positivity. A cross check across reference regions can also be used to
 1188 screen for reference region reliability.

Commented [DM4]: Edison P, Hinz R, Ramlackhansingh A, Thomas J, Gelosa G, Archer HA, Turkheimer FE, Brooks DJ. Can target-to-pons ratio be used as a reliable method for the analysis of [11C]PIB brain scans? Neuroimage. 2012 Apr 15;60(3):1716-23. doi: 10.1016/j.neuroimage.2012.01.099. Epub 2012 Jan 27.

Commented [DM5]: Blautzik J, Brendel M, Sauerbeck J, Kotz S, Scheiwein F, Bartenstein P, Seibyl J, Rominger A; Alzheimer's Disease Neuroimaging Initiative. Reference region selection and the association between the rate of amyloid accumulation over time and the baseline amyloid burden. Eur J Nucl Med Mol Imaging. 2017 Aug;44(8):1364-1374.

Commented [DM6]: Chen K, Roontiva A, Thiyayagura P, Lee W, Liu X, Ayutyanont N, Protas H, Luo JL, Bauer R, Reschke C, Bandy D, Koeppe RA, Fleisher AS, Caselli RJ, Landau S, Jagust WJ, Weiner MW, Reiman EM; Alzheimer's Disease Neuroimaging Initiative. Improved power for characterizing longitudinal amyloid-β PET changes and evaluating amyloid-modifying treatments with a cerebral white matter reference region. J Nucl Med. 2015 Apr;56(4):560-6. Landau SM, Breault C, Joshi AD, Pontecorvo M, Mathis CA, Jagust WJ, Mintun MA; Alzheimer's Disease Neuroimaging Initiative. Amyloid-β imaging with Pittsburgh compound B and florbetapir: comparing radiotracers and quantification methods. J Nucl Med. 2013 Jan;54(1):70-7.

Landau SM, Fero A, Baker S.L., Koeppe R., Mintun M., Chen K., Reiman, E.M., Jagust, W.J. Measurement of Longitudinal B Amyloid Change with 18F Florbetapir PET and Standardized Uptake Value Ratios. J. Nucl. Med. 2015;56, 567-574. Schwarz CG, Senjem ML, Gunter JL, Tosakulwong N, Weigand SD, Kemp BJ, Spychalla AJ, Vemuri P, Petersen RC, Lowe VJ, Jack CR Jr. Optimizing PIB-PET SUVR Change-Over-Time Measurement by a large-scale analysis of Longitudinal Reliability, Plausibility, Separability, and Correlation with MMSE. Neuroimage. 2016 Aug 27. pii: S1053-8119(16)30448-7. Shokouhi S, Mckay JW, Baker SL, Kang H, Brill AB, Gwirtsman HE, Riddle WR, Claassen DO, Rogers BP; Alzheimer's Disease Neuroimaging Initiative. Reference tissue normalization in longitudinal (18)F-florbetapir positron emission tomography of late mild cognitive impairment. Alzheimers Res Ther. 2016

Abstracts and Presentations
 Fleisher, A.S., Roontiva, A., Reschke, C., Bandy, D., Reiman, E.M., Protas, H., Luo, J., Chen, K., Weiner, M.W., Ayutyanont, N., Thiyayagura, P., Caselli, R.J., Baur, R.L., Koeppe, R., Landau, S., Lee, W., Jagust, W., Liu, X. Improving the Power to Track Fibrillar Amyloid PET Measurements and Evaluate Amyloid Modifying

Commented [DM7]: Tryputsen V, DiBernardo A, Samtani M, Novak GP, Narayan VA, Raghavan N; Alzheimer's Disease Neuroimaging Initiative. Optimizing regions-of-interest composites for capturing treatment effects on brain amyloid in clinical trials. J Alzheimers Dis. 2015;43(3):809-21. doi: 10.3233/JAD-131979.

Landau SM, Fero A, Baker SL, Koeppe R, Mintun M, Chen K, Reiman EM, Jagust WJ. Measurement of longitudinal β-amyloid change with 18F-florbetapir PET and standardized uptake value ratios. J Nucl Med. 2015 Apr;56(4):567-74. doi: 10.2967/jnumed.114.148981. Epub 2015 Mar 5.

Commented [DM8]: Tryputsen V, DiBernardo A, Samtani M, Novak GP, Narayan VA, Raghavan N; Alzheimer's Disease Neuroimaging Initiative. Optimizing regions-of-interest composites for capturing treatment effects on brain amyloid in clinical trials. J Alzheimers Dis. 2015;43(3):809-21. doi: 10.3233/JAD-131979.

Landau SM, Fero A, Baker SL, Koeppe R, Mintun M, Chen K, Reiman EM, Jagust WJ. Measurement of longitudinal β-amyloid change with 18F-florbetapir PET and standardized uptake value ratios. J Nucl Med. 2015 Apr;56(4):567-74. doi: 10.2967/jnumed.114.148981. Epub 2015 Mar 5.

Parameter	Entity/Actor	Specification
Reference Region Definition	Image Analyst	The reference region definition will conform to protocol by including the specified tissue. Quality control measures will be applied to ensure that longitudinal change is not attributable to technical noise

Parameter	Entity/Actor	Specification
		or artifact in a particular reference region.

1190

1191 3.4.3.2.3 Apply Regions to Subject Scans for Measurement

1192 Target VOIs may be applied for measurement either to the non-intensity normalized image, or to an SUVR
 1193 image that was first generated by dividing each voxel by the average value in the reference region. When
 1194 placing VOIs, it is critical to ensure accurate fit, and that only appropriate tissue is included. Potential
 1195 sources of error include the following:

1196

1197 Differences in tissue composition: Positioning of a cortical VOI toward the edge of gray matter in one scan
 1198 vs. toward white matter in a second longitudinal scan will introduce measurement error due to the tissue
 1199 composition and partial volume effects. In cross-sectional measurement, these differences can also be
 1200 significant for subjects at threshold of positivity.

1201

1202 Tissue truncation: If the scan does not have a complete cerebellum or other region, and the VOI samples
 1203 the empty space, a large error can result depending upon proportion of missing tissue for the VOI.

1204

1205 Differences in tissue sampled: Measuring different portions of tissue (e.g., the full region in one scan vs.
 1206 only a part of the region due to tissue truncation in the second scan) across longitudinal scans can
 1207 introduce errors of a few to several percent.

1208

Parameter	Entity/Actor	Specification
Region placement	Image Analyst	The placement of all regions of interest and reference region(s) will be verified to be on the correct tissue
Region placement	Image Analyst	All regions will be checked to ensure that boundaries do not include empty space (scan truncation). Regions will be adjusted using a consistent approach, such as automated exclusion of voxels, with a sub-threshold value, to exclude voxels where tissue is missing.
Region placement	Image Analyst	The same portion of tissue will be measured between longitudinal scans for the same subject.

1209

1210 3.4.3.2.4 Generate SUVR Image

1211 Once a reference region has been applied to the scan, and either before target region measurement, or
 1212 afterward, a SUVR image (or DVR in the case of a fully dynamic scan) can optionally be generated by
 1213 dividing each voxel value by the reference region mean.

1214

1215 This is useful for visual comparison and evaluation of images, regardless of which regions are to be
 1216 measured quantitatively. Once an SUVR image has been generated, target VOIs can also be applied and
 measured without further division by a reference region value.

1217

1217 3.4.3.3 Create SUVR

3.4.3.3.1 Measure Regional Values

The mean value within each VOI is calculated as the numerator for the SUVR. A cortical average may be calculated as the average of multiple VOIs, or weighted by the number of voxels in each VOI. While the selection of which regions to include and how to combine them is dependent upon the study objectives, minimizing variation due to numerous technical factors (including subject motion, axial variability, and image alignment) is best achieved when using an average of multiple regions. The performance claim is derived from published studies in which a non-weighted average of cingulate, frontal, lateral temporal, and lateral parietal regions was applied.

Formatted: Justified

3.4.3.3.2 Calculate SUVR

The SUVR is calculated by dividing the VOI value by the reference region value (which will be 1.0 if measured on a SUVR image). If a parametric image was generated using full dynamic scanning, or if a kinetic model is being applied to a multi-timeframe dynamic image, a DVR value is generated instead.

3.4.3.3.3 Relating SUVR values to other studies: the Centiloid

Different protocols involve different tracers, target regions, and reference regions, and all of these contribute to how the SUVR can be interpreted with regard to amyloid burden. A value of 1.2, for example, can be amyloid positive using one tracer and/or set of regions for analysis, but amyloid negative using a different tracer and/or regions. In order to reconcile findings across data acquisition, processing, and analysis protocols, the concept of the Centiloid was developed (Klunk et al, 2015; Rowe et al, 2013). The Centiloid is not intended to dictate the method for acquiring and processing data, but rather to provide a way to equate results obtained with a broad variety of protocol parameters. The basis for the Centiloid is a “gold standard” set of results derived from young healthy controls and elderly AD patients. These results have been generated using the radiotracer 11C-PiB and a defined set of target region, reference region, and image processing and analysis steps. A linear progression of values from 0 (no amyloid) to 100 (mean for amyloid positive sporadic AD patients) has been established using these values this approach. To establish the equivalent “Centiloid value” for a tracer and/or acquisition and analysis protocol that differ from the gold standard, two sets of relationships are required to be empirically derived. Using the control image set provided by the Centiloid project, it is first confirmed that by using the prescribed regions and analysis approaches, the Centiloid values can be generated—replicated with a correlation (r^2) exceeding 0.98 exceeding 98%. Secondly, using the new tracer and/or acquisition and analysis parameters, values are generated using both the “gold standard” method and 11C-PiB, and the alternate tracer and/or methods. The regression between the two sets of results yields a transform equation that can be applied to results to convert them to “Centiloid units” for comparison to other studies. If a tracer and set of approaches are being applied that for which conversion to Centiloid units has already been established, this reference transform can be directly applied to new studies using the same conversion parameters. PiB, flutemetamol, florbetaben and other image, SUVR and conversion data are available on the GAAIN website: <http://www.gaain.org/centiloid-project>.

It is noted that while the Centiloid can be used to reconcile values across tracers and methods, its use does not change the within-method variability or error that is already present (Su et al, 2018).

3.4.4 Required Characteristics of Resulting Data

The specific trial protocol shall prospectively define the SUVR (regions to be measured, which regions are to

1259 be included in a cortical average if applicable, and how the average is to be calculated) that is required for
 1260 the imaging endpoint. SUVr measures and the analysis tools used to obtain them, including software
 1261 version shall be specified for each protocol and shall be used consistently across all subjects and across all
 1262 sequential measurements.

1263 It should be clear which values belong to which brain region. Reports must clearly associate the region,
 1264 including any hemispheric reference, with the measured value via column headers or other information
 1265 display. Correct association of value and region should be assured via documentation that may include
 1266 audit log via software that has been validated to correctly produce this information, DICOM coordinates
 1267 captured along with the SUV, provision of the sampling “masks” or boundaries used to make the
 1268 measurements for each subject, or secondary screen captures of the ROI for identification. The volume of
 1269 each region measured, in voxels that can be translated into cc, or in cc, should also be included, along with
 1270 the minimum, maximum, and standard deviation within the region mentioned.

1271 The reference tissue (e.g., cerebellum (whole or gray), pons, subcortical white matter, combination, other)
 1272 must be reported along with the target region SUV data. Identification should be specific, indicating
 1273 whether gray, white, or both tissue types were included, and which slices were included or excluded.

1274 The analysis software should generate a report that is clear, traceable, and interpretable.

1275 3.5. Image Interpretation and Reporting

1276 ~~No QIBA Profile specification can be provided for image interpretation at this time. Image Interpretation is~~
 1277 ~~considered to be beyond the scope of this document.~~In the context of this quantitative Profile,
 1278 interpretation refers to the way in which the quantitative SUVr or DVR measurements are used, rather
 1279 than to a visual interpretation of the scan. Reporting of SUVr or DVR values is subject to the requirements
 1280 of the study.

1281 ~~In other words, how quantitative response is measured should be specified a priori by the trial itself. This~~
 1282 ~~also applies to target lesion selection.~~

Parameter	Entity/Actor	Specification
Image Reporting	Imaging Facility	Imaging reports shall be populated from DICOM header information using structured reportings <u>shall conform to the requirements of the study protocol.</u>

1285 3.6. Quality Control

1286 The following section deals with multiple aspects of quality control in amyloid-PET studies. This includes
 1287 selecting and qualifying a PET/CT imaging facility, imaging personnel and PET/CT scanners and ancillary
 1288 equipment. In addition, the use of phantom imaging (prior to study initiation and ongoing) is discussed as
 1289 well as identifying subjects whose data may need to be censored due to a lack of data integrity. Finally,
 1290 post-image-acquisition quality assessment is detailed.

1291 3.6.1 Imaging Facility

1292 It is essential to implement quality processes that ensure reliable performance of the scanner and

1293 consistent image acquisition methodology. These processes must be in place prior to subject imaging and
 1294 be followed for the duration of the trial. A facility “imaging capability assessment” is a prerequisite to
 1295 facility selection for participation in any clinical trial involving the use of amyloid-PET/CT as an imaging
 1296 biomarker. This imaging capability assessment will include:

- 1297 • Identification of appropriate imaging equipment intended for use in the trial
- 1298 • Documented performance of required quality control procedures of the scanner and ancillary
 1299 equipment (e.g., radionuclide calibrator)
- 1300 • Radiotracer quality control procedures
- 1301 • Experience of key personnel (technologists, radiologists, physicists and/or other imaging experts)
- 1302 • Procedures to ensure imaging protocol conformance during the trial

1303 **3.6.1.1 Site Accreditation/Qualification Maintenance**

1304 Whilst imaging facility accreditation is generally considered to be adequate for routine clinical practice
 1305 purposes (e.g., ACR, IAC, and TJC), facility qualification (e.g., EARL, SNMMI-CTN, ACRIN, and imaging core
 1306 labs) -may be required for clinical research/clinical trial participation. In order to be considered to be
 1307 conformant with this Profile, an imaging scanner/facility must provide documentation of current qualified
 1308 status. Appropriate forms, checklists or other process documents should be maintained and presented
 1309 upon request to verify that ongoing quality control procedures are being performed in a timely manner as
 1310 dictated by specific clinical study requirements. If exceptions to any of the performance standards stated
 1311 below occur and cannot be remediated on site, the site should promptly communicate the issue to the
 1312 appropriate internal overseer for advice as to how the irregularity should be managed. In addition to
 1313 documenting the level of performance required for this Profile (and the level of performance achieved), the
 1314 frequency of facility accreditation/qualification also needs to be described.

1315 It is important to note that that imaging facility Accreditation and/or Qualification, as defined in this Profile,
 1316 are considered necessary, but are not sufficient for being conformant with this Profile. In order to be
 1317 conformant with the Profile, and thus to support the claims of the Profile, all normative requirements must
 1318 be met.

Parameter	Entity/Actor	Specification
Accreditation / Qualification	Imaging Site & Image Acquisition Device	Shall maintain and document Accredited status for clinical practice (ACR, IAC, TJC, etc.) or Qualified status for clinical trials (e.g. ACRIN, SNMMI-CTN, EARL, iCROs, etc.).

1319 **3.6.2 Imaging Facility Personnel**

1320 For each of the personnel categories described below, there should be training, credentialing, continuing
 1321 education and peer review standards defined. Guidelines for training/credentialing for each resource
 1322 category are summarized below (UPICT Protocol Section 2.1). Note that only physicians reading the PET/CT
 1323 amyloid scans need specific training and certification for PET amyloid interpretation.

Parameter	Entity/Actor	Specification
-----------	--------------	---------------

Parameter	Entity/Actor	Specification
Personnel Roster	Imaging Facility Coordinator	Each site shall, at the time of trial activation and prior to subject accrual, have the support of certified technologists, physicists, and physicians (as defined below), experienced in the use of amyloid-PET/CT in the conduct of clinical trials.
Technologist	Imaging Facility Coordinator	Technologist certification shall be equivalent to the recommendations published by the representatives from the Society of Nuclear Medicine <u>and Molecular Imaging</u> Technologists Section (SNM <u>MI</u> -TS) and the American Society of Radiologic Technologists (ASRT) and should also meet all local, regional, and national regulatory requirements for the administration of ionizing radiation to patients.
Medical Physicist	Imaging Facility Coordinator	Medical physicists shall be certified in Medical Nuclear Physics or Radiological Physics by the American Board of Radiology (ABR); in Nuclear Medicine Physics by the American Board of Science in Nuclear Medicine (ABSNM); in Nuclear Medicine Physics by the Canadian College of Physicists in Medicine; or equivalent certification in other countries; or have performed at least two annual facility surveys over the last 24 months.
Physician	Imaging Facility Coordinator	Physicians overseeing PET/CT scans shall be qualified by the <u>have board certification by the American Board of Nuclear Medicine (ABNM) and/or the American Board of Radiology (ABR) ABR</u> (Diagnostic and/or Nuclear Radiology) or American Board of Nuclear Medicine (ABNM) or equivalent within the United States or an equivalent entity appropriate for the geographic location in which the imaging study(ies) will be performed and/or interpreted. Physicians interpreting the scans should have appropriate, specific initial training in interpretation of amyloid brain PET studies (specific to the PET amyloid tracer being used) and maintain continuing proficiency as outlined by national imaging professional societies, appropriate for the geographic location in which imaging studies are performed.

1325

1326 **3.6.3 Amyloid- PET Acquisition Scanner**

1327 Amyloid-PET studies as described in this Profile require either a PET/CT scanner or a dedicated PET scanner
 1328 with the ability to acquire a transmission image. PET/MR scanners may be added in future versions of this
 1329 Profile or may already be included in this Profile if the repeatability of the SUVRs from these scanners is
 1330 conformant with the assumptions underlying the claims.~~PET/MR scanners may be added in future versions~~
 1331 ~~of this Profile.~~ The scanners should be identified based on manufacturer, name and model. Hardware
 1332 specifications should be documented. Scanner software name and version should be documented at the
 1333 time of trial initiation and at the time of any and all updates or upgrades.

1334 The scanner must undergo routine quality assurance and quality control processes (including preventive
 1335 maintenance schedules) appropriate for clinical applications, as defined by professional and/or regulatory
 1336 agencies. In order to assure adequate quantitative accuracy and precision of imaging results, additional
 1337 quality assurance measures are required, as discussed below.

1338 For consistency, clinical trial subjects should be imaged on the same device over the entire course of a
 1339 study. A replacement scanner of the same make and model may be used if it is properly qualified. It is
 1340 imperative, however, that the trial sponsor be notified of scanner substitution if it occurs.

1341 For clinical trials with quantitative imaging requirements, a subject should have all scans performed on only
 1342 one scanner unless quantitative equivalence with a replacement scanner can be clearly demonstrated.
 1343 However, it should be noted that there are currently no accepted criteria for demonstrating quantitative
 1344 equivalence between scanners. It is anticipated that future version of this Profile will provide such criteria.

1345

Parameter	Entity/Actor	Specification
Physical Inspection	Technologist	Shall, on a daily basis, check gantry covers in tunnel and subject handling system.
QA/QC Checks	Technologist	At a minimum, QA/QC procedures shall be performed each day according to vendor recommendations. Daily QC procedures shall be performed prior to any subject scan.

1346 **3.6.3.1 Ancillary Equipment**

1347 3.6.3.1.1 Radionuclide Calibrator

1348 The following guidelines are collected from ANSI standard N42.13, 2004 and IAEA Technical Report Series
 1349 TRS-454. All requirements assume measurements on unit doses of amyloid tracer and that calibration
 1350 sources are in the 'syringe' geometry (i.e., no bulk doses).

1351 The Constancy test ensures reproducibility of an activity measurement over a long period of time by
 1352 measuring a long-lived source of known activity.

1353 The Accuracy test ensures that the activity values determined by the radionuclide calibrator are correct and
 1354 traceable to national or international standards within reported uncertainties.

1355 The Linearity test confirms that, for an individual radionuclide, the same calibration setting can be applied
 1356 to obtain the correct activity readout over the range of use for that radionuclide calibrator.

Parameter	Entity/Actor	Specification
Constancy	Technologist	Shall be evaluated daily (or after any radionuclide calibrator event) using a NIST-traceable (or equivalent) simulated ¹⁸ F, Cs-137, or Co-57 radionuclide calibrator standard and confirmed that net measured activity differs by no greater than ±2.5 % from the expected value.

Parameter	Entity/Actor	Specification
Accuracy	Technologist	Shall be evaluated monthly (or after any radionuclide calibrator event) with a NIST-traceable (or equivalent) simulated F-18 radionuclide calibrator standard. Shall confirm that net measured activities differ no greater than $\pm 2.5\%$ from expected value.
		The scanner calibration shall be tested using a NIST-traceable (or equivalent) simulated 18F source object, e.g. a uniform cylinder, large enough to avoid partial volume effects or other resolution losses.
Linearity	Technologist or Radiation safety officer or Qualified Medical Physicist	Shall be evaluated annually (or after any radionuclide calibrator event) using either 18F or Tc-99m and should be within $\pm 2.5\%$ of the true value over an operating range of 37-1110 MBq (1 to 30 mCi) and the true value is determined by a linear fit (to the log data) over the same operating range.
PET Radiation Dose	Dose Calibrator	Shall record the radiation dose from the administered activity and accompanying information in a DICOM Radiopharmaceutical Administration Radiation Dose Structured Report.

1357

1358 3.6.3.1.2 Scales and stadiometers

1359 Scales and stadiometers should be inspected and calibrated at installation and annually.

1360

Parameter	Entity/Actor	Specification
Scales	Approved personnel	Shall be evaluated annually or after any repair by qualified personnel. Shall be confirmed that error is less than $\pm 2.5\%$ from expected values using NIST-traceable or equivalent standards.

1361

1362 3.6.3.1.4 Clocks and timing devices

1363 The PET and CT scanner computers and all clocks in an imaging facility used to record activity/injection
 1364 measurements should be synchronized to standard time reference within ± 1 minute. These include any
 1365 clocks or timekeeping systems that are connected with a subject's amyloid-PET study, in particular those
 1366 associated with the radionuclide calibrator, the injection room, the scanner, and the acquisition
 1367 computer(s). The synchronization of all clocks (to date, time of day and to time zone) should be monitored
 1368 periodically as part of ongoing QA program. In particular, clocks should be inspected immediately after
 1369 power outages or civil changes for Daylight Savings (NA) or Summer Time (Eur). Correct synchronization
 1370 could be achieved using the Consistent Time Integration Profile as defined in the IHE IT Infrastructure
 1371 Technical Framework. The Consistent Time Profile requires the use of the Network Time Protocol (NTP)
 1372 (www.NTP.org).

Parameter	Entity/Actor	Specification
Scanner and site clocks	Approved personnel	PET and CT scanner computers and all clocks in an Imaging facility used to record activity/injection measurements shall be synchronized to standard time reference within +/-1 minute. Synchronization of all clocks used in the conduct of the amyloid-PET study shall be checked weekly and after power outages or civil changes for Daylight Savings (NA) or Summer Time (Eur)
Scanner and site clocks	Specific Device	Provide time synchronization as per the IHE Consistent Time Integration Profile.
Dose calibrator clock	Dose Calibrator	Electronic record of output from a dose calibrator shall be synchronized with other time keeping devices.

1373

1374 **3.6.4 Phantom Imaging**1375 **3.6.4.1 Uniformity and Calibration**

1376 Verification of scanner normalization with a uniform phantom is a minimum requirement for all scanners
 1377 used in clinical trials including those that only have qualitative endpoints. A Hoffman or equivalent
 1378 phantom may be used in place of a uniform phantom to verify scanner normalization via in-plane and axial
 1379 comparisons to an analytical gold standard for that phantom over the complete field of view to be used by
 1380 the amyloid ~~measurand~~ measurement. For trials with quantitative PET measurements, this assessment
 1381 should also include a comparison against a radionuclide calibrator to ensure quantitative accuracy; that is, a
 1382 comparison of the absolute activity measured versus the measured amount injected should be performed.
 1383 This comparison is particularly important after software or hardware upgrades. If the trial requires absolute
 1384 quantification in baseline images or absolute changes in longitudinal studies, it should be considered to
 1385 include an image quality and/or contrast recovery QC assessment as part of the routine QC procedures
 1386 and/or scanner validation process. Clinical trials using only relative changes in longitudinal studies may not
 1387 require contrast recovery assessments provided there is appropriate consideration for the minimum size of
 1388 target lesions based on the partial volume effect.

1389 An essential requirement for extracting quantitative data from images is that there be known calibration
 1390 accuracy and precision and/or cross calibration of the PET system against the (locally) used radionuclide
 1391 calibrator (within 10%). The QC procedures should utilize the same acquisition/reconstruction protocol,
 1392 software and settings that are used for the subject scans.

1393

Parameter	Entity/Actor	Specification
Phantom tests: Frequency of uniformity measurements	Imaging Site	Shall perform at baseline, quarterly and after scanner upgrades, maintenance or repairs, and new setups.
Uniformity QC	Technologist	At least quarterly and following software upgrades, shall

Parameter	Entity/Actor	Specification
		<p>assess transverse and axial uniformity across image planes by imaging a uniform cylinder phantom.</p> <ol style="list-style-type: none"> 1. Visual check that no streak artifacts or axial plane non-uniformities are present. 2. The standard deviation of a large central 2D ROI (<u>3D when drawn on multiple slices</u>) shall be compared with similar previous scans to check for measurable differences. 3. The mean values of a large central 2D ROI for all image slices (<u>resulting in a 3D VOI</u>) shall be compared with similar previous scans to check for measurable differences.
Phantom tests: transaxial uniformity measurement	Imaging Site	Shall measure the transaxial (within plane) uniformity as specified in NEMA NU2 1994; uniformity should be $\leq 10\%$ for each qualified axial slice (see below).
		Shall measure the transaxial (within plane) uniformity as specified in NEMA NU2 1994; uniformity should be $\leq 5\%$ for each qualified axial slice (see below).
Phantom tests: axial uniformity measurement	Imaging Site	Shall measure the axial uniformity by placing a circular ROI that is at least 1 cm in diameter less than the active diameter of the cylinder phantom, centered on each of the axial planes. Calculate the COV (std dev/mean * 100) of each ROI. Axial planes whose COV is $\leq 10\%$ qualify for use (e.g. some of the end planes may not qualify). (<u>Note that if the historical 10% tolerance is applied rather than 1%, a similar error can be introduced into longitudinal SUVR measurement and the reference region and target region must be in the same axial slices from scan to scan.</u>)
		Shall measure the axial uniformity using the same procedure as above, except axial planes whose COV is $\leq 5\%$ qualify for use.
		Harmonized image reconstruction protocols are available. (i.e., known recovery coefficients versus size for a given test object such as the modified NEMA NU-2 Image Quality phantom.

1394

1395 **3.6.4.2 Resolution**

1396 The assessment of adequate resolution should include both a qualitative evaluation (using clinical or
1397 anthropomorphic phantom images) and quantitative assessment (using phantom-defined criteria).

Parameter	Entity/Actor	Specification
Resolution	Nuclear Medicine	Shall perform, on at least an annual basis, and document a qualitative resolution QC test by using the manufacturer's

Parameter	Entity/Actor	Specification
	Physician	settings and demonstrating resolution of normal gross anatomic features within clinical images of the brain.
Resolution	Medical Physicist	Shall perform (during an initial site qualification process, and then at least every one year) and document performance of a quantitative assessment (using a phantom with differing size defined targets such as the Hoffman, ACR or NEMA IQ phantoms) for spatial resolution.
		Follow the modified procedure developed by Lodge et al. [JNM 2009; 50:1307-1314] to use a slightly tilted uniform phantom to get axial and in-plane spatial resolution.

1398

1399 **3.6.4.3 Noise**

Parameter	Entity/Actor	Specification
Phantom tests: Frequency of noise measurements	Imaging Site	Shall perform at baseline, quarterly and after scanner upgrades, maintenance or repairs, and new setups.
Phantom test: noise measurements	Medical Physicist	A uniform cylinder phantom or equivalent shall be filled with an 18-F concentration in the uniform area (approximately 0.1 to 0.2 $\mu\text{C}/\text{ml}$), and scanned using the intended acquisition protocol. Using a rectangular or spherical region as close as possible to, but no smaller than, 3 cm to a side, the COV of the voxel values within the region should be below 15%, for the slices within the central 80% of the axial FOV.

1400

1401 **3.6.4.3.4 Amyloid-PET Specific Phantom Measurements**

1402 The above more general phantom evaluations of a PET scanner are needed to qualify it for clinical practice
 1403 or a clinical trial. However, more purpose-specific phantoms are also needed to simulate the human brain,
 1404 amyloid uptake patterns, and the amyloid SUVR measurand. Purpose-specific phantom options that might
 1405 be considered on a per-protocol basis include, but are not limited to:

- 1406 1. Each site uses a single phantom for the duration of the trial but not necessarily the same model of
 1407 phantom used at other sites.
- 1408 2. All sites use phantoms of the same model for the duration of the trial.
- 1409 3. All sites use phantoms built to precise specifications for the duration of the trial.
- 1410 4. All sites share a single phantom for the duration of the trial.

1411 The phantom scans and performance evaluation should be performed prior to the start of a trial and
 1412 repeated during the course of the trial as specified by the individual protocol. Any changes to scanner

1413 equipment, either hardware or software, should be immediately reported to the trial sponsor and/or
1414 imaging CRO and may result in the need for re-qualification prior to imaging additional trial subjects. In
1415 particular, it is strongly recommended that subjects in a longitudinal study be scanned on the same PET
1416 system with the same software version whenever possible.

1417 Generally, the purpose-specific phantom scans must provide a metric to characterize these imaging
1418 properties:

- 1419 • Spatial resolution – PET scanner hardware, reconstruction methods and reconstruction parameter
1420 selections can result in dramatically different spatial resolutions in the reconstructed images.
1421 Because partial volume effects (especially between gray and white matter regions) can bias many
1422 amyloid PET measurands, it is essential to calibrate the spatial resolution of each scanner using the
1423 acquisition and reconstruction protocol planned for patient imaging. A post-reconstruction
1424 smoothing operation can then be applied for calculation of a measurand at a uniform spatial
1425 resolution between scanners.
- 1426 • Uniformity – In-plane and axial uniformity of the purpose-specific phantom should be within 10%
1427 throughout the scanner field of view to be used in the calculation of the amyloid PET measurand.
1428 Note that the historical axial uniformity tolerance of 10% has the implication that if a subject is
1429 imaged in one axial location for one scan, and in a different axial location (e.g. a few cm different)
1430 for the next scan, then the slices used to calculate each reference or target region value may change
1431 DIFFERENTLY. This can introduce error of a few percent to many percent into the longitudinal SUVR
1432 change. Selection of reference region and target region in the same axial slices can help to mitigate
1433 this potential source of noise, as the differences cancel out.
- 1434 • Absence of reconstruction artifacts – Reconstructed purpose-specific phantom data should be
1435 visually free of reconstruction artifacts, such as streaks due to failing detectors or axial plane non-
1436 uniformities due to errors in normalization.
- 1437 • Qualitative and quantitative accuracy – Measurands using ratios, such as the SUVR must
1438 demonstrate accuracy with 10% of an analytical or otherwise known gold standard.

1439 An anthropomorphic phantom, such as the 3D Hoffman phantom or equivalent, ideally with a spatial
1440 distribution similar to the cortical gray/white matter is required to characterize the five imaging properties
1441 listed above. A uniform phantom or a point source phantom by themselves is not adequate to sufficiently
1442 characterize the amyloid imaging properties of a PET scanner. The phantom should be adequate to model
1443 and characterize effects of attenuation correction and scatter correction. Contrast ratios of amyloid tracer
1444 uptake vary between normal and abnormal subjects, and also between different amyloid tracers. However,
1445 it is recommended that the phantom be filled such that the activity concentration in the highest uptake
1446 regions be similar to the expected white matter uptake in subjects with amyloid deposition. For the
1447 Hoffman phantom, it is recommended that the activity at the start of the scan be 0.5-0.6 mCi (18.5-22.2
1448 MBq) to obtain approximately a 15 kBq/ml activity in the gray matter regions of the phantom. See
1449 Appendix H for best practices guidance for this phantom.

1450 The Hoffman phantom should be centered in the FOV of the PET scanner and data acquired for 20 minutes.
1451 Moreover, image reconstruction methods and settings should equal those specified in the study. The post-
1452 processing and data analysis should be as similar as possible to those used with patient data.

1453 A baseline assessment of the scanner imaging properties is required before any subjects are scanned in the
1454 trial, and after any major hardware or software modifications that could affect these properties. Following

Formatted: Underline

1455 a baseline qualification assessment using the Hoffman phantom, routine manufacturer-recommended QA
 1456 procedures (e.g. daily QC checks, quarterly normalization, etc.) using simpler phantoms may be adequate to
 1457 demonstrate acceptable scanner performance over the course of a clinical trial. A baseline qualification
 1458 assessment is required at least annually in an extended study.

1460 The normative list below is based on the Hoffman anthropomorphic, NEMA Image Quality, ACR, and
 1461 uniform cylinder phantoms as appropriate.

Parameter	Entity/Actor	Specification
Phantom tests: Frequency of measurements based on Hoffman phantom data	Imaging Site	Needed as an initial baseline characterization and thereafter annually as well as after major scanner upgrades, maintenance or repairs.
Phantom test: resolution measurement	Imaging Site	Acquire data using the Hoffman phantom and compute the FWHM "Hoffman equivalent" [Joshi/Koeppel NeuroImage 46 (2009) 154-159] FWHM resolution, in transverse and axial directions. The resolution should be <= 8.0 mm FWHM.
Phantom test: gray/white matter ratio measurement	Imaging Site	Register the Hoffman phantom PET image to the digital representation of the phantom, and compute the gray/white matter ratio. This ratio should be > 0.55. See Appendix I for more details.
Phantom test: SUVR accuracy	Imaging Site	Using the Hoffman phantom PET image perform the same post-processing and image analysis to confirm the SUVR accuracy. See Appendix I for more details.

1464 3.6.4.4.5 Phantom imaging data analysis

1465 For amyloid-PET image analysis, there are many combinations of hardware and software that are used. The
 1466 software alone comprises multiple layers including the operating system, several base modules for input
 1467 and display, and the components that draw/calculate ROIs and calculate the SUVR. See Section 4.4 and
 1468 Appendix F.

1470 3.6.5 Quality Control of Amyloid-PET studies

1471 3.6.5.1 Data Integrity

1472 The integrity of DICOM image headers should be reviewed and confirmed for DICOM standard compliance,
 1473 regulatory compliance (including privacy protection, such as may be required by such rules as the HIPAA
 1474 Privacy Rule if applicable), protocol compliance, sufficiency for the intended analysis (e.g., to compute SUV)
 1475 and consistency with source data such as CRFs.

3.6.5.2 Determination of Image Quality

CT and 68-Ge transmission images should be reviewed by the Image Analyst for assessment of image quality and for potential artifacts such as beam hardening, metal objects, and motion. PET images should be compared to the transmission images for proper image registration and potential attenuation correction artifacts. Both uncorrected and attenuation corrected images may need to be assessed to identify any artifacts caused by contrast agents, metal implants and/or subject motion. For example, movement or mis-registration can lead to poor quality quantitative data and invalid numbers. Some images may be too poor in quality to quantify. Statistical quality of images is important to report, but not a full substitute for quality.

~~3.6.5.3 Determination of subjects unsuitable for Amyloid PET analysis~~

~~3.6.6 Quality Control of Interpretation~~

~~To promote quantifiable performance standards for the quality control of interpretation there is a need for intra-reader variability studies. In a two-Reader paradigm, then inter-reader variability is needed as well. It is currently unclear what statistics to evaluate and how these performance metrics should be used in the analysis.~~

Formatted: Normal, Left

4. Conformance Procedures

Relation of this Profile to Expectations for QIBA Profile Conformance

Definitions (from Appendix C):

Qualified: The imaging site is formally approved by an appropriate body (i.e., ACRIN, CQIE, SNM-CTN, EANM-EARL, an imaging laboratory or CRO) for a specific clinical research study.

Accredited: Approval by an independent body or group for broad clinical usage (requires ongoing QA/QC) e.g., ACR, IAC, TJC.

Conformant: The imaging site and equipment meet all the requirements described herein, which are necessary to meet the QIBA Profile claim.

The requirements included here are intended to establish a baseline level of capabilities. Providing higher levels of performance or advanced capabilities is both allowed and encouraged. Furthermore, the QIBA Profile is not intended to limit equipment suppliers in any way with respect to how they meet these requirements. Institutions meeting the stated criteria are considered to be QIBA Conformant.

4.1. Performance Assessment: Image Acquisition Site

Typically, clinical sites are selected due to their competence in neurology and access to a sufficiently large subject population under consideration. For imaging sites, it is important to have availability of:

- Appropriate imaging equipment and quality control processes,
- Appropriate ancillary equipment and access to radiotracer and contrast material,
- Experienced Technologists (CT and PET trained) for the subject handling and imaging procedure,

- 1511 • Appropriately trained Radiologists/Nuclear Medicine Physicians for image analysis and diagnostic
1512 interpretation,
 - 1513 • Appropriately trained image analysts, with oversight by a Radiologist or Nuclear Medicine Physician,
 - 1514 • Medical Physics support to ensure appropriate scanner and equipment calibration, and to address
1515 issues relating to quantification such as attenuation maps or movement
 - 1516 • Processes that assure imaging QIBA Profile-conformant image generation in appropriate time window
- 1517 A QA/QC program for PET scanners and ancillary devices must be in place to achieve the goals of the
1518 clinical trial. The minimum requirements are specified above. This program shall include (a) elements to
1519 verify that imaging facilities are performing imaging studies correctly and (b) elements to verify that
1520 facility's PET scanners are performing within specified calibration values. These may involve additional
1521 PET and CT phantom testing that address issues relating to both radiation dose and image quality
1522 (which may include issues relating to water calibration, uniformity, noise, spatial resolution – in the
1523 axial plane-, reconstructed slice thickness z-axis resolution, contrast scale, and others) and constancy.
1524 There is agreement that some performance testing (e.g. constancy phantom) adds value; however,
1525 acceptable performance levels, frequency of performance, triggers for action and mitigation strategies
1526 need further definition before these can be required. This phantom testing may be done in addition to
1527 the QA program defined by the device manufacturer as it evaluates performance that is specific to the
1528 goals of the clinical trial.

1529

Parameter	Entity/Actor	Specification
PET Scanner	Acquisition Facility	This Profile shall only address full ring PET scanners that have the capability of acquiring a transmission image for attenuation correction and have a minimum axial FOV of 15 cm for a single bed position.
CT Scanner Calibration	Technologist	Shall perform daily water equivalent phantom analysis; ensure that output is acceptable and manually enter on form /electronic database.
PET Scanner Calibration	Technologist	Shall perform daily/weekly/monthly scanner QA and vendor recommended maintenance procedures (e.g., replace weak transmission sources for dedicated PET scanner); ensure that output values are acceptable and manually enter on form/electronic database
PET Scanner Calibration Constancy Check	Technologist	Shall perform constancy phantom (e.g., for example, a Ge-68 cylinder <u>if applicable</u>) scan (preferably NIST traceable or equivalent to gather information regarding uniformity as well) at least weekly and after each calibration.
Radionuclide calibrator		Calibrated to 18F using NIST traceable source or equivalent either by site or calibrator manufacturer.

1530

1531 **4.2. Performance Assessment: PET Acquisition Device**

1532 Distinct from the performance specifications and frequency of testing described in Section 4.1, which apply
1533 to quality control of the Acquisition Device at the imaging facility, this Section defines performance
1534 specifications of the Acquisition Device to be met upon leaving the manufacturing facility. In order to be in
1535 conformance with this Profile, the Acquisition Device should be held to the same standard whether a
1536 mobile utility or a fixed installation; a mobile scanner may require additional calibration to achieve this
1537 performance.

1538 The PET scanner should use DICOM attributes to follow version numbers of software for: 1 Acquisition, 2
1539 Reconstruction, 3 Post-processing, 4 Display/ROI analysis, 5 Dynamic Analysis. Performance requirements
1540 regarding software version identification, documentation and tracking across time are described in Section
1541 4.5.

1542 The PET scan acquisition start time should be used for the decay reference time and the integral model
1543 should be used for decay correction. The scanner should perform all decay corrections (i.e. not the
1544 operator). Image data are to be given in units Bq/ml. "Derived" images (distinct from "Original") should be
1545 flagged following the DICOM standard and should retain the scan acquisition date and time fields.

1546 All needed information for fully corrected administered activity (e.g., residual activity, injection time,
1547 calibration time) is required. Note that use of the term administered activity below refers to fully corrected
1548 net radioactivity.

1550 Baseline level conformance requires that the DICOM image set from the subject's PET scan and necessary
1551 metadata (that is not currently captured by all PET scanner acquisition processes) is captured in trial
1552 documentation, e.g., case report forms. The metadata is required to perform the quantitative analysis and
1553 perform quality control on SUV covariates. This includes for example, post-injection residual activity and
1554 subject height. This data should be captured in the 'Common Data Format Mechanism' as described in
1555 Appendix E.

1557 The DICOM format used by the PET scanner should meet the Conformance Statement written by
1558 manufacturer of the PET system. PET data shall be encoded in the DICOM PET or Enhanced PET Image
1559 Storage SOP Class, and in activity-concentration units (Bq/ml) with additional parameters in public DICOM
1560 fields to calculate SUVs (e.g., height, weight, scale factors). CT data should be encoded in CT or Enhanced CT
1561 Image Storage SOP Class. DICOM data shall be transferred using the DICOM Part 8 network protocol or as
1562 offline DICOM Part 10 files for media storage including CDs and DVDs. They shall be transferred without any
1563 form of lossy compression.

1564 The meta-information is the information that is separate, or in addition to, the image values (in units of
1565 Bq/ml) that is deemed necessary for quantitatively accurate representation of PET SUVs. The meta-
1566 information may also include other information beyond that need for calculation of SUVs, i.e. the type and
1567 or sequencing of therapy, the blood glucose levels, the scanner SUV stability history, etc. The actual
1568 mechanism of capturing the information is not specified in this Profile. The intent here is to list what
1569 information should be captured rather than the mechanism itself. The mechanism can range from paper
1570 notes, to scanned forms or electronic data records, to direct entry from the measurement equipment into
1571 pre-specified DICOM fields (i.e., from the PET scanner or auxiliary measurement devices such as the
1572 radionuclide calibrator). Ideally all of the specified meta-data will be captured by direct electronic entry to
1573 DICOM fields, after suitable modification of the DICOM format for PET imaging.

1574 In some facility workflows, the Acquisition Device may also provide workstation/analysis tool functionality.

1575 For example, the display of an SUV statistic (considered in Section 4.4.1) or display of Tracer Uptake Time
 1576 (considered in Section 4.4), may also apply to the Acquisition Device, if used in this manner.

1577 The concept endorsed here is that the needed meta-data is identified. Through revisions of this Profile, the
 1578 DICOM standard, and technology the meta-data is inserted into the analysis stream (Figure 3) in a more
 1579 direct manner and technology and accepted standards evolve.

1580

Parameter	Entity/Actor	Specification
CT calibration tracking	Acquisition Device	Daily water equivalent phantom values shall be tracked in the DICOM header.
PET calibration factor	Acquisition Device	The current SUV calibration factor shall be included in the DICOM header.
PET QA status	Acquisition Device	Date/time and status of system-wide QA checks should be captured separately.
Radionuclide calibrator calibration	Acquisition Device	Calibration factor for an F-18 NIST -traceable (or equivalent) source with identifying information shall be tracked in the DICOM header with Date/Time.
PET Scanner calibration	Acquisition Device	<p>Shall be able to be calibrated according to the following specifications:</p> <ul style="list-style-type: none"> Using an ACR type uniform cylinder containing F-18 in water (ideally the same used for dose calibrator cross-calibration) Using a long scan time of 60 min or more (to minimize noise), and an ACR-type ROI analysis <p>The average measured SUV shall be in the range of 0.98 to 1.02. (Note this is not the performance expected during clinical imaging operation as discussed in preamble to this Section).</p> <p>Slice-to-slice variability shall be no more than $\pm 5\%$. (not including end slices, as per ACRPET Core Lab).</p> <p>In-plane uniformity for above phantom shall be less than 5 %.</p>
Weight	Acquisition Device	<p>Shall be able to record patient weight in lbs or kg as supplied from the modality worklist and/or operator entry into scanner interface. Shall be stored in Patient Weight field (0010,1030) in the DICOM image header, as per DICOM standard.</p> <p>Patient weight shall be specifiable with 4 significant digits.</p> <p>Patient weight shall be transferrable directly from measurement device into scanner by electronic, HIS/RIS, or other means, bypassing all operator entry, but still permitting operator correction.</p>
BMI	Acquisition	Depending upon the study requirements, BMI shall be specified.

Formatted Table

Parameter	Entity/Actor	Specification
	Device	
Height	Acquisition Device	<p>Shall be able to record patient height in feet/inches or cm/m as supplied from the modality worklist and/or operator entry into scanner interface. Shall be stored in Patient Size field (0010,1020) in the DICOM image header, as per DICOM standard.</p> <p>Patient height shall be specifiable with 3 significant digits.</p> <p>Patient height shall be transferrable directly from measurement device into scanner by electronic, HIS/RIS, or other means, bypassing all operator entry, but still permitting operator correction.</p>
Administered Radionuclide	Acquisition Device	<p>Shall be able to accept the radionuclide type (i.e., F-18) from the DICOM Modality Worklist either from the NM/PET Protocol Context, if present, or by deriving it from the Requested Procedure Code via a locally configurable tables of values.</p> <p>Shall be able to enter the radionuclide type (i.e., F-18) by operator entry into the scanner interface.</p> <p>Shall be recorded in Radionuclide Code Sequence (0054,0300) in the DICOM image header (e.g., (C-111A1, SRT, “¹⁸Fluorine”).</p> <p>Shall be able to accept the radionuclide type (i.e., F-18) directly from the measurement device (dose calibrator) or management system, using the Sup 159 Radiopharmaceutical Administration Radiation Dose Report bypassing all operator entry, but still permitting operator correction.</p>
Administered Radiotracer	Acquisition Device	<p>Shall be able to record the specific radiotracer as supplied by operator entry into the scanner interface. Shall be recorded in Radionuclide Code Sequence field (0054,0300) in the DICOM image header, e.g., (C-B1031, SRT, “Fluorodeoxyglucose F¹⁸”).</p>
Administered Radiotracer radioactivity	Acquisition Device	<p>Shall be able to enter the administered radioactivity, in both MBq and mCi, as supplied by operator entry into the scanner interface. Shall be recorded in Radionuclide Total Dose field (0018,1074) in the DICOM image header in Bq.</p> <p>Shall be able to record with separate entry fields on scanner interface:</p> <ol style="list-style-type: none"> (1) the pre-injection ¹⁸F-Amyloid tracer radioactivity (2) time of measurement of pre-injection ¹⁸F-Amyloid tracer radioactivity (3) the residual activity after injection (4) time of measurement the residual radioactivity after injection <p>Shall automatically calculate the administered radioactivity and store</p>

Parameter	Entity/Actor	Specification
		<p>in the Radionuclide Total Dose field (0018,1074) in the DICOM image header.</p> <p>Alternatively, shall be able to receive this information as per DICOM Supplement 159.</p> <p>Patient Administered Radiotracer radioactivity information shall be transferred directly from measurement device into scanner by electronic, HIS/RIS, or other means, bypassing all operator entry, but still permitting operator correction.</p>
Administered Radiotracer Time	Acquisition Device	<p>Shall be able to record the time of the start of activity injection as supplied by operator entry into the scanner interface. Shall be recorded in Radiopharmaceutical Start Date Time field (0018,1078) (preferred) or Radiopharmaceutical Start Time field (0018,1072).</p> <p>Shall be able to record the time of the start of activity injection as supplied by operator entry into the scanner interface. Shall be recorded in Radiopharmaceutical Start Date Time field (0018,1078). I.e. not Radiopharmaceutical Start Time field (0018,1072).</p> <p>Shall be able to record the time of the stop of activity injection as supplied by operator entry into the scanner interface. Shall be recorded in Radiopharmaceutical Stop Date Time field (0018,1079).</p>
Decay Correction Methodology	Acquisition Device	<p>Encoded voxel values with Rescale Slope field (0028,1053) applied shall be decay corrected by the scanner software (not the operator) to a single reference time (regardless of bed position), which is the start time of the first acquisition, which shall be encoded in the Series Time field (0008,0031) for original images.</p> <p>Corrected Image field (0028,0051) shall include the value "DECY" and Decay Correction field (0054,1102) shall be "START", which means that the images are decay corrected to the earliest Acquisition Time (0008, 0032).</p>
Scanning Workflow	Acquisition Device	<p>Shall be able to support Profile Protocol (Section 3) PET and CT order(s) of acquisition.</p> <p>Shall be able to pre-define and save (by imaging site) a Profile acquisition Protocol for patient acquisition.</p> <p>Shall be able to interpret previously-reconstructed patient images to regenerate acquisition protocol.</p> <p>Shall be configurable to store (or receive) acquisition parameters as pre-defined protocols (in a proprietary or standard format), to allow re-use of such stored protocols to meet multi-center specifications and to achieve repeatable performance across time points for the same subject.</p>

Parameter	Entity/Actor	Specification
CT Acquisition Parameters	Acquisition Device	Shall record all key acquisition parameters in the CT image header, using standard DICOM fields. Includes but not limited to: Actual Field of View, Scan Duration, Scan Plane, Total Collimation Width, Single Collimation Width, Scan Pitch, Tube Potential, Tube Current, Rotation Time, Exposure and Slice Width in the DICOM image header.
CT based attenuation correction	Acquisition Device	Shall record information in PET DICOM image header which CT images were used for corrections (attenuation, scatter, etc.).
PET-CT Alignment	Acquisition Device	Shall be able to align PET and CT images within ± 2 mm in any direction.
		Shall be able to align PET and CT images within ± 2 mm in any direction under maximum load over the co-scan length.
CT Absorbed Radiation Dose	Acquisition Device	Shall record the absorbed dose (CTDI, DLP) in a DICOM Radiation Dose Structured Report.
Activity Concentration in the Reconstructed Images	Acquisition Device	Shall be able to store and record (rescaled) image data in units of Bq/ml and use a value of BQML for Units field (0054,1001).
Tracer Uptake Time	Acquisition Device	Shall be derivable from the difference between the Radiopharmaceutical Date Time field (0018,1078) (preferred) or Radiopharmaceutical Start Time field (0018,1072) and the Series Time field (0008,0031) or earliest Acquisition Time field (0008,0032) in the series (i.e., the start of acquisition at the first bed position), which should be reported as series time field (0008,0031).
PET Voxel size	Acquisition Device	See Section 4.3 (PET Voxel size) under the Reconstruction Software specification requirements.
CT Voxel size	Acquisition Device	Shall be no greater than the reconstructed PET voxel size. Voxels shall be square, although are not required to be isotropic in the Z (head-foot) axis. Not required to be the same as the reconstructed PET voxel size.
Subject Positioning	Acquisition Device	Shall be able to record the subject position in the Patient Orientation Code Sequence field (0054,0410) (whether prone or supine) and Patient Gantry Relationship Code field Sequence (0054,0414) (whether head or feet first).
Scanning Direction	Acquisition Device	Shall be able to record the scanning direction (craniocaudal vs. caudocranial) into an appropriate DICOM field.
Documentation	Acquisition	Shall be able to record and define the x-y axis FOV acquired in Field of

Parameter	Entity/Actor	Specification
of Exam Specification	Device	View Dimensions (0018,1149) and reconstructed in Reconstruction Diameter (0018,1100). Shall be able to define the extent of anatomic coverage based on distance from defined landmark site (e.g., vertex, EAM). (both the landmark location (anatomically) and the distance scanned from landmark) would require DICOM tags). Shall be able to be reportable for future scanning sessions. The Acquisition Device shall record the z-axis FOV which represents the actual distance of scan anatomic coverage (cm).
Differential Acquisition Time	Acquisition Device	Shall be able to acquire and record non uniform scan times dependent upon areas of clinical concern. Recording can be done through the use of Actual Frame Duration (0018,1242) and Frame Reference Time (0054, 1300).
<u>Events</u>	<u>Acquisition Device</u>	<u>Shall record any events such as patient stopped scanning session or got up out of scanner during scanning session. (These events are to be recorded on the scanning session CRF at a minimum.)</u>
DICOM Compliance	Acquisition Device	All image data and scan parameters shall be transferable using appropriate DICOM fields according to the DICOM conformance statement for the PET scanner.
DICOM Data transfer and storage format	PET Scanner or Display Workstation	PET images shall be encoded in the DICOM PET or Enhanced PET Image Storage SOP Class, using activity-concentration units (Bq/ml) with additional parameters stored in public DICOM fields to enable calculation of SUVs. PET images shall be transferred and stored without any form of lossy compression.

Formatted Table

1581

Parameter	Entity/Actor	Specification
DICOM Editing	Acquisition Device	Shall be able to edit all fields relevant for SUV calculation before image distribution from scanner. Shall provide appropriate warnings if overriding of the current values is initiated.

1582

1583

4.3. Performance Assessment: Reconstruction Software

1584

Reconstruction Software shall propagate the information collected at the prior Subject Handling and Imaging Acquisition stages and extend it with those items noted in the Reconstruction section.

1585

Parameter	Entity/Actor	Specification
-----------	--------------	---------------

Parameter	Entity/Actor	Specification
Metadata	Reconstruction Software	Shall be able to accurately propagate the information collected at the prior stages and extend it with those items noted in the Reconstruction section.

Data can be reconstructed including all corrections needed for quantification as well as without scatter and attenuation correction. Analytical or iterative reconstruction methods should be applied. If the system is capable of providing resolution recovery and/or time of flight, then the decision to 'turn on' or 'turn off' this/these capabilities should be made prospectively, as dictated by the specific protocol, and should be consistent for a given subject across multiple time points.

Standardization of reconstruction settings is necessary to obtain comparable resolution and SUV recoveries across the same subject and inter-subject across sites.

Parameter	Entity/Actor	Specification
Data Corrections	Reconstruction Software	PET emission data must be able to be corrected for geometrical response and detector efficiency, system dead time, random coincidences, scatter and attenuation.
Reconstruction Methodology	Reconstruction Software	Shall be able to provide iterative and/or analytical (e.g., filtered back projection) reconstruction algorithms.
		Shall be able to indicate, for both TOF and Resolution recovery, if either is being used for purposes of image reconstruction.
Reconstruction Methodology / Output	Reconstruction Software	Shall be able to perform reconstructions with and without attenuation correction.
Data Reconstruction 2D/3D Compatibility	Reconstruction Software	Shall be able to perform reconstruction of data acquired in 3D mode using 3D image reconstruction algorithms. If 3D mode data can be re-binned into 2D mode, shall be able to perform reconstruction of data acquired in 3D mode using 2D image reconstruction algorithms.
Quantitative calibration	Reconstruction software	Shall apply appropriate quantitative calibration factors such that all images have units of activity concentration, e.g., kBq/mL.
Voxel size	Reconstruction software	Shall allow the user to define the image voxel size by adjusting the matrix dimensions and/or diameter of the reconstruction field-of-view.
		Shall be able to reconstruct PET voxels with a size 2.5 mm or less in the transaxial directions and 2.5 mm or less in the axial dimension (as

Parameter	Entity/Actor	Specification
		<p>recorded in Voxel Spacing field (0028,0030) and computed from the reconstruction interval between Image Position (Patient) (0020,0032) values of successive slices).</p> <p>Pixels shall be square, although voxels are not required to be isotropic in the z (head-foot) axis.</p>
		<p>Shall be able to reconstruct PET voxels with a size of 2 mm or less in all three dimensions (as recorded in Voxel Spacing field (0028,0030) and computed from the reconstruction interval between Image Position (Patient) (0020,0032) values of successive slices).</p> <p>Voxels shall be isotropic.</p>
Reconstruction parameters	Reconstruction software	<p>Shall allow the user to control image noise and spatial resolution by adjusting reconstruction parameters, e.g., number of iterations, post-reconstruction filters.</p>
		<p>Shall be able to record reconstruction parameters used in image DICOM header using the Enhanced PET IOD, developed by DICOM working group.</p>
Reconstruction protocols	Reconstruction software	<p>Shall allow a set of reconstruction parameters to be saved and automatically applied (without manual intervention) to future studies as needed.</p>

4.3. Performance Assessment: Image Analysis Workstation

4.4. Performance Assessment: Image Analysis Workstation

Currently, there is no commercially available tool with which image analysis workstation conformance can be assessed. Versions of a Hoffmann brain DRO have been used by some labs to perform some of the necessary tasks, but not all requirements, as defined in this Profile can be assessed with this/these DROs.

A digital reference object (DRO) series of synthetic PET volumes derived from a single patient's MRI scan (also provided) shall be used to evaluate conformance of the image analysis workstation (IAW). Users should use the DRO series (as per the DRO user's guide in Appendix F) to verify correct implementation of VOI placement for both target and reference regions, SUVR calculations, PET alignment to standardized atlases (when applicable), system linearity and system reproducibility.

Parameter	Entity/Actor	Specification
Performance Evaluation	Image Analyst & Analysis Workstation	Shall use the DRO series to verify adequate performance as described in Appendix F and save the results with any study compliant with this Profile.
Repeatability	Image Analysis	Shall be validated to achieve repeatability with a within-subject CV of less than or equal to 2.6%. See Appendix F.

Parameter	Entity/Actor	Specification
	Workstation	
	Image Analyst	Shall, if operator interaction is required by the Image Analysis Workstation tool to perform measurement, be validated to achieve repeatability with a within-subject CV of less than or equal to 2.6%. See Appendix F.
Linearity	Image Analysis Workstation	Shall be validated to achieve: <ul style="list-style-type: none"> slope (\hat{A}_1) between 0.95 and 1.05 R-squared (R^2) >0.90 See Appendix F.

1607

1608 The post-processing software, which may be integral to the scanner workstation or provide by a third-party
 1609 vendor, shall have the ability to perform the operations specified in Section 3.3.2, Image Data Post-
 1610 processing.

Parameter	Entity/Actor	Specification
Metadata	Image Post-processing workstation	Shall be able to accurately propagate the information collected at the prior stages and extend it with those items noted in the Image Analysis Workstation section. Shall be able to display all information that affects SUVRs either directly in calculation (e.g., region of interest intensity) or indirectly (image acquisition parameters).
Image acquisition parameters: Display	Image Post-processing workstation	Shall be capable to display or include link to display the number of minutes between injection and initiation of imaging (as per derivation guidelines described in Section 4.2), and the duration of each timeframe in cases where the image consists of multiple timeframes.

1611

1612 The Image Post-processing workstation will allow for the following operations that may or may not have
 1613 been performed as part of image reconstruction.
 1614

Parameter	Entity/Actor	Specification
Decay correction	Image Post-processing workstation	Shall allow for image decay correction if not performed during reconstruction. Shall use either the Acquisition Time field (0008,0032) or Radiopharmaceutical Start Time (0018,1072), if necessary. If a series (derived or not) is based on Acquisition Time decay correction, the earliest Acquisition Time (0008,0032) shall be used as the reference time for decay correction.
Image	Image Post-processing	Shall allow user to orient image per protocol in x, y, and z

Parameter	Entity/Actor	Specification
orientation	workstation	directions.
Intra-scan, inter-frame alignment	Image Post-processing workstation	Shall be able to automatically spatially align the different timeframes that may have been acquired
Intra-scan, inter-frame alignment	Image Post-processing workstation	Shall allow selection of an anchor frame to which other frames are aligned
Intra-scan, inter-frame alignment	Image Post-processing workstation	Shall measure and display the translational and rotational parameters necessary to align each frame to the reference frame.
Static image creation	Image Post-processing workstation	Shall allow exclusion of one or more frames from the static image that is created through frame averaging or summation
Static image creation	Image Post-processing workstation	Shall be able to sum and/or average the selected timeframes to create a static image for analysis
Smoothing	Image Post-processing workstation	Shall be able to apply a 3D smoothing filter if indicated as part of study protocol
Data storage and transfer	Image Post-processing workstation	Shall be able to store images after each major step of image manipulation (e.g., after frame summation)

1615
1616
1617
1618
1619
1620
1621

The features required of the analysis workstation are dependent in part upon the methods chosen for definition and application of the target and reference regions of interest to the PET scan. Certain additional features such as kinetic modeling for full dynamic scans, partial volume correction, and MRI segmentation to create regions of interest may also be relevant per study protocol, but their description is beyond the scope of this document.

Parameter	Entity/Actor	Specification
Image Quality control: Visual inspection	Image Analysis workstation	Shall be able to display each image in a manner such that all image slices in the transaxial, sagittal, and coronal views may be examined visually.
Spatial mapping: Image fusion (co-registration)	Image Analysis workstation	Shall be able to automatically and accurately spatially align the PET image with the subject's MRI scan in cases where this approach is implemented.
Spatial mapping: Co-registration between visits	Image Analysis workstation	Shall be able to automatically and accurately spatially align multiple PET visits to one another when this approach is implemented.
Spatial Mapping: warp	Image Analysis	Shall be able to automatically and accurately spatially map the subject's scan and template to each other when this

Parameter	Entity/Actor	Specification
to template	workstation	approach is implemented.
Target and reference region definition	Image Analysis workstation	Shall provide either the means for defining target and reference region of interest boundaries to be applied to the subject scan, or for importing pre-defined region of interest boundaries (or masks) that may have been generated using other software (such as generated through segmentation of subject's MRI or pre-defined based upon an image template and atlas).
SUVR image creation	Image Analysis workstation	Shall be able to create an SUVR image by dividing each voxel by the average value within a selected reference region, if this option is implemented.
Region placement	Image Analysis workstation	Shall be able to apply (place for measurement) pre-specified regions of interest onto the PET scan in an anatomically accurate manner.
Region placement quality control	Image Analysis workstation	Shall allow means for quality assurance that regions for measurement have been accurately placed on the PET scan (either by final region placement inspection and/or inspection and/or automatic quality measurements performed at each image manipulation step)
Region of interest measurement	Image Analysis workstation	Shall be able to calculate the mean value within each region of interest, and store for SUVR calculations (if not based on an SUVR image) and/or reporting.
SUVR calculation	Image Analysis workstation	Shall be able to calculate SUVR values by dividing the mean value in a target region by the mean value in the reference region (if not based on an SUVR image).
SUVR output	Image Analysis workstation	Shall be able to store and output SUVR values for display and for transfer to a study report, to a precision as required by the study protocol.

4.3. Performance Assessment: Software Version Tracking

4.5. Performance Assessment: ~~Software version tracking~~

Ideally, the PET scanner should be able to build a list on the console of the dates of all software versions (software changes that might impact quantitative accuracy would typically be inclusive of hardware change). Furthermore, the scanner software version should be identified and tracked across time, with updates and changes in scanner software noted during the trial. At a minimum, Software Versions should be manually recorded during the qualification along with the phantom imaging performance data and the record should be updated for every software-upgrade over the duration of the trial. This includes the flagging of the impact on quantification for now; in the future, record all software version numbers in DICOM header.

Parameter	Entity/Actor	Specification
Software Version tracking	Acquisition Device	Shall record the software version(s) used for acquisition and reconstruction in appropriate DICOM field(s).
Software version back-testing compatibility	Workstation	Shall provide mechanism to provide analysis of the image data using updated as well as prior (platform-specific) versions of analysis software.

References

Test-Retest Papers & Methodology

Inter-scan period less than 60 days

- Joshi AD, Pontecorvo MJ, Clark CM, Carpenter AP, Jennings DL, Sadowsky CH, Adler LP, Kovnat KD, Seibyl JP, Arora A, Saha K, Burns JD, Lowrey MJ, Mintun MA, Skovronsky DM, Florbetapir F 18 Study Investigators. Performance Characteristics of Amyloid PET with Florbetapir F 18 in Patients with Alzheimer's Disease and Cognitively Normal Subjects. *J Nucl Med* 2012; 53:378-384, DOI: 10.2967/jnumed.111.090340.
- Vandenberghe R, Van Laere K, Ivanoiu A, Salmon E, Bastin C, Triau E, Hasselbalch S, Law I, Andersen A, Korner A, Minthon L, Garraux G, Nelissen N, Bormans G, Buckley C, Owenius R, Thurfjell L, Farrar G, Brooks DJ. 18F-Flutemetamol Amyloid Imaging in Alzheimer Disease and Mild Cognitive Impairment A Phase 2 Trial. *Ann Neurol* 2010;68:319-329, DOI: 10.1002/ana.22068.

Two-year period

- Brendel M, Högenauer M, Delker A, Sauerbeck J, Bartenstein P, Seibyl J, Rominger A; Alzheimer's Disease Neuroimaging Initiative. Improved longitudinal [(18)F]-AV45 amyloid PET by white matter reference and VOI-based partial volume effect correction. *Neuroimage*. 2015 Mar;108:450-9. doi: 10.1016/j.neuroimage.2014.11.055.
- Chen K, Roontiva A, Thiyagura P, Lee W, Liu X, Ayutyanont N, Protas H, Luo JL, Bauer R, Reschke C, Bandy D, Koeppe RA, Fleisher AS, Caselli RJ, Landau S, Jagust WJ, Weiner MW, Reiman EM; Alzheimer's Disease Neuroimaging Initiative. Improved power for characterizing longitudinal amyloid-β PET changes and evaluating amyloid-modifying treatments with a cerebral white matter reference region. *J Nucl Med*. 2015 Apr;56(4):560-6.

(See also Schwarz below as a review of other comparisons of longitudinal variability)

- Clinical Validation of 18F-AZD4694, an Amyloid-β-Specific PET Radioligand, Zsolt Csele'nyi, Maria Eriksdotter Joh'nhagen, Anton Forsberg, Christer Halldin, Per Julin, Magnus Schou, Peter Johnstro'm, Katarina Varna's, Samuel Svensson, and Lars Farde, *J Nucl Med* 2012; 53:415-424, DOI: 10.2967/jnumed.111.094029.
- Performance Characteristics of Amyloid PET with Florbetapir F 18 in Patients with Alzheimer's Disease and Cognitively Normal Subjects, Abhinay D. Joshi, Michael J. Pontecorvo, Christopher M. Clark, Alan P. Carpenter, Danna L. Jennings, Carl H. Sadowsky, Lee P. Adler, Karel D. Kovnat, John P. Seibyl, Anupa Arora, Krishnendu Saha, Jason D. Burns, Mark J. Lowrey, Mark A. Mintun, Daniel M. Skovronsky, and the Florbetapir F-18 Study Investigators, *J Nucl Med* 2012; 53:378-384, DOI: 10.2967/jnumed.111.090340.

Formatted: Font: Italic

Formatted: Font: Italic

Formatted: Indent: Left: 0", Hanging: 0.31", Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

Formatted: Comment Text, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

Formatted: Comment Text, Space Before: 6 pt

Formatted: Space Before: 6 pt, After: 0 pt

3. [18F-Flutemetamol Amyloid Imaging in Alzheimer Disease and Mild Cognitive Impairment A Phase 2 Trial](#), Rik Vandenberghe, MD, hD, Koen Van Laere, MD, PhD, Adrian Ivanoiu, MD, PhD, Eric Salmon, MD, PhD, Christine Bastin, PhD, Eric Triau, MD, Steen Hasselbalch, MD, DMSc, Ian Law, MD, PhD, Allan Andersen, MD, Alex Korner, MD, PhD, Lennart Minthon, MD, Gae"tan Garraux, MD, PhD, Natalie Nelissen, PhD, Guy Bormans, PhD, Chris Buckley, MD, Rikard Owenius, Lennart Thurfje, Gill Farrar, PhD, and David J. Brooks, MD, DSc, FRCP, *ANN NEUROL* 2010;68:319–329, DOI: 10.1002/ana.22068. *Eur J Nucl Med Mol Imaging* (2009) 36:1629–1638, DOI 10.1007/s00259-009-1129-6.

Formatted: Justified, Space Before: 6 pt, After: 0 pt

4. [Test-retest variability of quantitative \[11C\] PIB studies in Alzheimer's disease](#). Nelleke Tolboom, Maqsood Yaqub, Ronald Boellaard, Gert Luurtsema, Albert D. Windhorst, Philip Scheltens, Adriaan A. Lammertsma, Bart N. M. van Berckel.

Formatted: Comment Text

5. [Longitudinal Assessment of A \$\beta\$ and Cognition in Aging and Alzheimer Disease](#), Victor L. Villemagne, Kerryn E. Pike, Gaël Chételat, Kathryn A. Ellis, Rachel S. Mulligan, Pierrick Bourgeat, Uwe Ackermann, Gareth Jones, Cassandra Szoek, Olivier Salvado, Ralph Martins, Graeme O'Keefe, Chester A. Mathis, William E. Klunk, David Ames, Colin L. Masters, and Christopher C. Rowe. *Ann Neurol*. 2011 January ; 69(1): 181–192. doi:10.1002/ana.22248.

6. [Amyloid Imaging with 18F-Florbetaben in Alzheimer Disease and Other Dementias](#), Victor L. Villemagne, Kevin Ong, Rachel S. Mulligan, Gerhard Holl, Svetlana Pejaska, Gareth Jones, Graeme O'Keefe, Uwe Ackerman, Henri Tochon-Danguy, J. Gordon Chan, Cornelia B. Reininger, Lueder Fels, Barbara Putz, Beate Rohde, Colin L. Masters, and Christopher C. Rowe. *J Nucl Med* 2011; 52:1210–1217, DOI: 10.2967/jnumed.111.089730

7. [Test-retest variability of high and low SA \[18F\]BAY 94-9172 in Alzheimer's disease and normal ageing](#). C. C. Rowe, S. Pejaska, R. Mulligan, G. Chan, L. Fels, H. Kusi, 2 C. Reininger, 2 B. Rohde, 2 B. Putz, V. L. Villemagne. Poster presented at the Society of Nuclear Medicine Meeting, Salt Lake City, UT, 2009.

Amyloid Imaging Methodology Papers

Formatted: Font: Bold

1. [Barret O, Alagille D, Sanabria S, Comley RA, Weimer RM, Borroni E, Mintun M, Seneca N, Papin C, Morley T, Marek K, Seibyl JP, Tamagnan GD, Jennings D. Kinetic Modeling of the Tau PET Tracer 18F-AV-1451 in Human Healthy Volunteers and Alzheimer's Disease Subjects. *J Nucl Med*. 2016 Dec 1.](#)

Formatted: Normal, Justified

2. [Blautzik J, Brendel M, Sauerbeck J, Kotz S, Scheiwein F, Bartenstein P, Seibyl J, Rominger A; Alzheimer's Disease Neuroimaging Initiative. Reference region selection and the association between the rate of amyloid accumulation over time and the baseline amyloid burden. *Eur J Nucl Med Mol Imaging*. 2017 Aug;44\(8\):1364-1374.](#)

Formatted: Justified, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, After: 0 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

3. [Brendel M, Högenauer M, Delker A, Sauerbeck J, Bartenstein P, Seibyl J, Rominger A; Alzheimer's Disease Neuroimaging Initiative. Improved longitudinal \[\(18\)F\]-AV45 amyloid PET by white matter reference and VOI-based partial volume effect correction. *Neuroimage* 2015 Mar;108:450-9. doi: 10.1016/j.neuroimage.2014.11.055.](#)

4. [Chen K, Roontiva A, Thiyyagura P, Lee W, Liu X, Ayutyanont N, Protas H, Luo JL, Bauer R, Reschke C, Bandy D, Koeppe RA, Fleisher AS, Caselli RJ, Landau S, Jagust WJ, Weiner MW, Reiman EM; Alzheimer's Disease Neuroimaging Initiative. Improved power for characterizing longitudinal amyloid- \$\beta\$ PET changes and evaluating amyloid-modifying treatments with a cerebral white matter reference region. *J Nucl Med*. 2015 Apr;56\(4\):560-6.](#)

5. [Edison P, Hinz R, Ramlackhansingh A, Thomas J, Gelosa G, Archer HA, Turkheimer FE, Brooks DJ. *Can*](#)

- 1707 [target-to-pons ratio be used as a reliable method for the analysis of \[11C\]PIB brain scans?](#)
 1708 [Neuroimage. 2012 Apr 15;60\(3\):1716-23. doi: 10.1016/j.neuroimage.2012.01.099.](#)
- 1709 6. [Fleisher, A.S., Roontiva, A., Reschke, C., Bandy, D., Reiman, E.M., Protas, H., Luo, J., Chen, K., Weiner,](#)
 1710 [M.W., Ayutyanont, N., Thiyyagura, P., Caselli, R.J., Baur, R.L., Koeppe, R., Landau, S., Lee, W., Jagust, W.,](#)
 1711 [Liu, X. Improving the Power to Track Fibrillar Amyloid PET Measurements and Evaluate Amyloid](#)
 1712 [Modifying Treatments using a Cerebral White Matter Reference Region of Interest, in: Alzheimer's](#)
 1713 [Association International Conference \(AAIC\). Elsevier, Copenhagen, Denmark, 2014.](#)
- 1714 7. [Hahn A, Schain M, Erlandsson M, Sjolin P, James GM, Strandberg OT, Hagerstrom D, Lanzenberger R,](#)
 1715 [Jogi J, Olsson TG, Smith R, Hansson O. Modeling Strategies for Quantification of In Vivo \(18\)F-AV-1451](#)
 1716 [Binding in Patients with Tau Pathology. J Nucl Med. 2017 Apr;58\(4\):623-631. doi:](#)
 1717 [10.2967/jnumed.116.174508. Epub 2016 Oct 20. PubMed PMID: 27765859.](#)
- 1718 8. [Joshi A, Kennedy IA, Mintun M, Pontecorvo M, Navitsky MA, Devous MD. Measuring change in beta](#)
 1719 [amyloid burden over time using florbetapir PET and a subcortical white matter reference region, in:](#)
 1720 [Alzheimer's Association International Conference \(AAIC\). Elsevier, Copenhagen, Denmark, 2014.](#)
- 1721 9. [Klein G, Sampat M, Staewen D, Scott D, Suhy J. Comparative Assessment of SUVR Methods and](#)
 1722 [Reference Regions in Amyloid PET Studies. Alzheimer's Association International Conference \(AAIC\),](#)
 1723 [July 18-23, 2015, Washington, DC, USA.](#)
- 1724 10. [Koeppe R. Basic Principles and Controversies in PET Amyloid Imaging. Human Amyloid Imaging](#)
 1725 [Meeting, Miami Beach, Florida, USA, 2012. On-line at:](#)
 1726 [http://www.slideshare.net/justinpearsonlighting/koeppe-ppt.](#)
- 1727 11. [Landau SM, Breault C, Joshi AD, Pontecorvo M, Mathis CA, Jagust WJ, Mintun MA; Alzheimer's Disease](#)
 1728 [Neuroimaging Initiative. Amyloid- \$\beta\$ imaging with Pittsburgh compound B and florbetapir: comparing](#)
 1729 [radiotracers and quantification methods. J Nucl Med. 2013 Jan;54\(1\):70-7.](#)
- 1730 12. [Landau SM, Fero A, Baker SL, Koeppe R, Mintun M, Chen K, Reiman EM, Jagust WJ. Measurement of](#)
 1731 [longitudinal \$\beta\$ -amyloid change with 18F-florbetapir PET and standardized uptake value ratios. J Nucl](#)
 1732 [Med. 2015 Apr;56\(4\):567-74. doi: 10.2967/jnumed.114.148981. Epub 2015 Mar 5.](#)
- 1733 13. [Lundqvist R, Lilja J, Thomas BA, Lötjönen J, Villemagne VL, Rowe CC, Thurfjell L. Implementation and](#)
 1734 [validation of an adaptive template registration method for 18F-flutemetamol imaging data. J Nucl](#)
 1735 [Med. 2013 Aug;54\(8\):1472-8. There are several additional papers that pertain to PiB also, by the](#)
 1736 [Klunk/Price group at Pittsburgh.](#)
- 1737 14. [Makris NE, Huisman MC, Kinahan PE, Lammertsma AA, Boellaard R. Evaluation of strategies towards](#)
 1738 [harmonization of FDG PET/CT studies in multicentre trials: comparison of scanner validation phantoms](#)
 1739 [and data analysis procedures. Eur J Nucl Med Mol Imaging. 2013 Oct;40\(10\):1507-15.](#)
- 1740 15. [Matthews DC, Marendic B, Andrews RD, Lukic AS, Einstein S, Liu E, Margolin RA, Schmidt ME, ADNI.](#)
 1741 [Longitudinal amyloid measurement for clinical trials: A new approach to overcome variability. Human](#)
 1742 [Amyloid Imaging conference, Miami Beach, poster presentation, 2014.](#)
- 1743 16. [Pontecorvo MJ, Devous MD Sr, Navitsky M, Lu M, Salloway S, Schaerf FW, Jennings D, Arora AK,](#)
 1744 [McGeehan A, Lim NC, Xiong H, Joshi AD, Siderowf A, Mintun MA; 18F-AV-1451-A05 investigators.](#)
 1745 [Relationships between flortaucipir PET tau binding and amyloid burden, clinical diagnosis, age and](#)
 1746 [cognition. Brain. 2017 Mar 1;140\(3\):748-763. doi: 10.1093/brain/aww334.](#)
- 1747 17. [Schmidt ME, Chiao P, Klein G, Matthews D, Thurfjell L, Cole PE, Margolin R, Landau S, Foster NL, Mason](#)

NS, De Santi S, Suhy J, Koeppe RA, Jagust W; Alzheimer's Disease Neuroimaging Initiative. The influence of biological and technical factors on quantitative analysis of amyloid PET: Points to consider and recommendations for controlling variability in longitudinal data. *Alzheimers Dement*. 2015 Sep;11(9):1050-68. doi: 10.1016/j.jalz.2014.09.004.

18. Schwarz CG, Senjem ML, Gunter JL, Tosakulwong N, Weigand SD, Kemp BJ, Spychalla AJ, Vemuri P, Petersen RC, Lowe VJ, Jack CR Jr. Optimizing PiB-PET SUVR Change-Over-Time Measurement by a large-scale analysis of Longitudinal Reliability, Plausibility, Separability, and Correlation with MMSE. *Neuroimage*. 2016 Aug 27. pii: S1053-8119(16)30448-7.

19. Shcherbinin S, Schwarz AJ, Joshi A, Navitsky M, Flitter M, Shankle WR, Devous MD Sr, Mintun MA. Kinetics of the Tau PET Tracer 18F-AV-1451 (T807) in Subjects with Normal Cognitive Function, Mild Cognitive Impairment, and Alzheimer Disease. *J Nucl Med*. 2016 Oct;57(10):1535-1542. Epub 2016 May 5. PubMed PMID: 27151986.

20. Shokouhi S, Mckay JW, Baker SL, Kang H, Brill AB, Gwirtsman HE, Riddle WR, Claassen DO, Rogers BP; Alzheimer's Disease Neuroimaging Initiative. Reference tissue normalization in longitudinal (18)F-florbetapir positron emission tomography of late mild cognitive impairment. *Alzheimers Res Ther*. 2016

21. Thurfjell L et al. Automated Quantification of 18F-Flutemetamol PET Activity for Categorizing Scans as Negative or Positive for Brain Amyloid: Concordance with Visual Image Reads. *J Nucl Med* October 1, 2014 vol. 55 no. 10 1623-1628. doi: G610.2967/jnumed.114.142109

22. Tryputsen V, DiBernardo A, Samtani M, Novak GP, Narayan VA, Raghavan N; Alzheimer's Disease Neuroimaging Initiative. Optimizing regions-of-interest composites for capturing treatment effects on brain amyloid in clinical trials. *J Alzheimers Dis*. 2015;43(3):809-21. doi: 10.3233/JAD-131979.

Attenuation Correction

1. Abella M, A. M. Alessio, D. A. Mankoff, L. R. Macdonald, J. J. Vaquero, M. Desco, and P. E. Kinahan. *Phys. Med. Biol* May 2012; 57:9, 2477–2490. Accuracy of CT-based attenuation correction in PET/CT bone imaging.

Centiloid Papers

1. ~~1. THE CENTILOID SCALE: STANDARDIZATION OF AMYLOID IMAGING MEASURES~~, Christopher Rowe CC, William Klunk, Robert Koeppe, William Jagust, Michael Pontecorvo, Michael Devous, Marybeth Howlett, Daniel Skovronsky, Keith Johnson, Julie Price, Chet Mathis, Mark Mintun. *The Centiloid scale: Standardization of Amyloid Imaging Measures.* *Alzheimer's & Dementia: The Journal of the Alzheimer's Association* Volume 9, Issue 4, Supplement , Page P8, July 2013, doi:10.1016/j.jalz.2013.04.026.

2. Rowe CC, Doré V, Jones G, Baxendale D, Mulligan RS, Bullich S, Stephens AW, De Santi S, Masters CL, Dinkelborg L, Villemagne VL. 18F-Florbetaben PET beta-amyloid binding expressed in Centiloids. *Eur J Nucl Med Mol Imaging*. 2017 Nov;44(12):2053-2059.

3. Su Y, Flores S, Horneck RC, Speidel B, Vlassenko AG, Gordon BA, Koeppe RA, Klunk WE, Xiong C, Morris JC, Benzinger TLS. Utilizing the Centiloid scale in cross-sectional and longitudinal PiB PET studies. *NeuroImage: Clinical*. Epub April 2018.

Formatted: Font: Bold

Formatted: Justified, Space Before: 6 pt, After: 0 pt

Formatted: Justified, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, After: 0 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

Formatted: Font: Bold

Formatted: Justified, Space Before: 6 pt, After: 0 pt

Formatted: Indent: Left: 0", Hanging: 0.38", Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

1789

1790

1791 **Non-imaging DX Tests**

1792 1. ~~Plasma phospholipids identify antecedent memory impairment in older adults, Mark Mapstone, Amrita~~
 1793 ~~K-Cheema, Massimo S Fiandaca, Xiaogang Zhong, Timothy R Mhyre, Linda H MacArthur, William J Hall,~~
 1794 ~~Susan G Fisher, Derick R Peterson, James M Haley, Michael D Nazar, Steven A Rich, Dan J Berlau, Carrie B~~
 1795 ~~Peltz, Ming T Tan, Claudia H Kawas & Howard J Federoff, Nature Medicine advance online publication,~~
 1796 ~~March 2014, doi:10.1038/nm.3466.~~

1797 **List of Medicines in Development for Alzheimer's Disease**

1798 1. ~~Medicines in Development Alzheimer's Disease presented by America's Biopharmaceutical Research~~
 1799 ~~Companies (PhRMA), 2013 Report, <http://www.phrma.org/sites/default/files/Alzheimer's%202013.pdf>.~~

1800 **ADNI References (<http://www.adni-info.org/scientists/ADNIStudyProcedures.aspx>)**

1801 1. ~~1-ADNI II Procedures Manual- <http://www.adni-info.org/Scientists/Pdfs/adniproceduresmanual12.pdf>~~
 1802 2. ~~ADNI Protocol - http://www.adni-info.org/Scientists/Pdfs/ADNI2_Protocol_FINAL_20100917.pdf~~
 1803 3. ~~Review Articles - The Alzheimer's Disease Neuroimaging Initiative: Progress report and future plans~~
 1804 ~~Michael W. Weiner, Paul S. Aisen, Clifford R. Jack, Jr., William J. Jagust, John Q. Trojanowski, Leslie~~
 1805 ~~Shaw, Andrew J. Saykin, John C. Morris, Nigel Cairns, Laurel A. Beckett, Arthur Toga, Robert Green,~~
 1806 ~~Sarah Walter, Holly Soares, Peter Snyder, Eric Siemers, William Potter, Patricia E. Cole, Mark Schmidt;~~
 1807 ~~and the Alzheimer's Disease Neuroimaging Initiative Alzheimer's & Dementia 6 (2010) 202–211~~

1808 **Amyloid PET: Clinical**

1809 ~~1. Appropriate use criteria for amyloid PET: A report of the Amyloid Imaging Task Force, the Society of~~
 1810 ~~Nuclear Medicine and Molecular Imaging, and the Alzheimer's Association. Keith A. Johnson KA,~~
 1811 ~~Satoshi Minoshima S, Nicolaas I. Bohnen NJ, Kevin J. Donohoe KJ, Norman L. Foster NL, Peter~~
 1812 ~~Herscovitch P, Jason H. Karlawish JH, Christopher C. Rowe CC, Maria C. Carrillo MC, Dean M. Hartley~~
 1813 ~~DM, Saima Hedrick S, Virginia Pappas V, William H. Thies WH. Appropriate use criteria for amyloid PET:~~
 1814 ~~A report of the Amyloid Imaging Task Force, the Society of Nuclear Medicine and Molecular Imaging,~~
 1815 ~~and the Alzheimer's Association.~~

1816 1.

1817 ~~2. Update on Appropriate Use Criteria for Amyloid PET Imaging: Dementia Experts, Mild Cognitive~~
 1818 ~~Impairment, and Education. Keith A. Johnson KA, Satoshi Minoshima S, Nicolaas I. Bohnen NJ, Kevin~~
 1819 ~~Donohoe KJ, Norman L. Foster NL, Peter Herscovitch P, Jason H. Karlawish JH, Christopher C. Rowe CC,~~
 1820 ~~Saima Hedrick S, Virginia Pappas V, Maria C. Carrillo MC, and Dean M. Hartley DM. Update on~~
 1821 ~~Appropriate Use Criteria for Amyloid PET Imaging: Dementia Experts, Mild Cognitive Impairment, and~~
 1822 ~~Education. J Nucl Med 2013; 54:1011–1013. DOI: 10.2967/jnumed.113.127068.~~

1823 2.

1824 ~~3. Pending journal permission: Schmidt ME et al, Manuscript regarding Approaches to Reduce~~
 1825 ~~Variability in Amyloid Imaging — this manuscript will contain a list of references, all of which could be~~
 1826 ~~applicable~~

1827 4. ~~Book chapter: Schmidt ME, Matthews D, Andrews R, Mosconi L. Book chapter: Positron Emission~~
 1828 ~~Tomography in Alzheimer Disease: Diagnosis and Use ~~ad-as~~ Biomarker Endpoints. Chapter 5, p. 131-194.~~

Formatted: Indent: Left: 0", Hanging: 0.31"

Formatted: Comment Text, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.31" + Indent at: 0.56"

Formatted: Comment Text, Left

1829 Translational Neuroimaging – Tools for CNS Drug Discovery, Development, and Treatment, McArthur RA
 1830 editor, 2013, Academic Press. This, too, contains a comprehensive list of references.

- 1831 3.
- 1832 4. Medicines in Development Alzheimer’s Disease presented by America’s Biopharmaceutical Research
 1833 Companies (PhRMA), 2013 Report,
 1834 <http://www.phrma.org/sites/default/files/Alzheimer's%202013.pdf>.

1835 PET-MR Scanners

- 1836 1. Cecchin D, Barthel H, Poggiali D, Cagnin A, Tiepolt S, Zucchetta P, Turco P, Gallo P, Frigo AC, Sabri O, Bui-
 1837 F. A new integrated dual time-point amyloid PET/MRI data analysis method. Eur J Nucl Med Mol
 1838 Imaging. 2017 Jul 4. doi: 10.1007/s00259-017-3750-0. [Epub ahead of print] PubMed PMID: 28674847.
- 1839 2. Fuin N, Pedemonte S, Catalano OA, Izquierdo-Garcia D, Soricelli A, Salvatore M, Heberlein K, Hooker
 1840 JM, Van Leemput K, Catana C. PET/MRI in the Presence of Metal Implants: Completion of the
 1841 Attenuation Map from PET Emission Data. J Nucl Med. 2017 May;58(5):840-845. doi:
 1842 10.2967/jnumed.116.183343. Epub 2017 Jan 26. PubMed PMID: 28126884; PubMed Central PMCID:
 1843 PMC5414501.
- 1844 3. Hitz S, Habekost C, Fürst S, Delso G, Förster S, Ziegler S, Nekolla SG, Souvatzoglou M, Beer AJ, Grimmer
 1845 T, Eiber M, Schwaiger M, Drzezga A. Systematic Comparison of the Performance of Integrated Whole-
 1846 Body PET/MR Imaging to Conventional PET/CT for ¹⁸F-FDG Brain Imaging in Patients Examined for
 1847 Suspected Dementia. J Nucl Med. 2014 Jun;55(6):923-31. doi: 10.2967/jnumed.113.126813. Epub 2014
 1848 May 15. PubMed PMID: 24833495.
- 1849 4. Ladefoged CN, Law I, Anazodo U, St Lawrence K, Izquierdo-Garcia D, Catana C, Burgos N, Cardoso MJ,
 1850 Ourselin S, Hutton B, Mérida I, Costes N, Hammers A, Benoit D, Holm S, Juttukonda M, An H, Cabello J,
 1851 Lukas M, Nekolla S, Ziegler S, Fenchel M, Jakoby B, Casey ME, Benzinger T, Højgaard L, Hansen AE,
 1852 Andersen FL. A multi-centre evaluation of eleven clinically feasible brain PET/MRI attenuation
 1853 correction techniques using a large cohort of patients. Neuroimage. 2017 Feb 15;147:346-359. doi:
 1854 10.1016/j.neuroimage.2016.12.010. Epub 2016 Dec 14. PubMed PMID: 27988322.
- 1855 5. Su Y, Rubin BB, McConathy J, Laforest R, Qi J, Sharma A, Priatna A, Benzinger TL. Impact of MR-Based
 1856 Attenuation Correction on Neurologic PET Studies. J Nucl Med. 2016;57(6):913-7. doi:
 1857 10.2967/jnumed.115.164822. PubMed PMID: 26823562; PMCID: PMC4891225.
- 1858 6. Werner P, Rullmann M, Bresch A, Tiepolt S, Jochimsen T, Lobsien D, Schroeter ML, Sabri O, Barthel H.
 1859 Impact of attenuation correction on clinical [(18)F]FDG brain PET in combined PET/MRI. EJNMMI Res.
 1860 2016 Dec;6(1):47. doi: 10.1186/s13550-016-0200-0. Epub 2016 Jun 3. PubMed PMID: 27255510;
 1861 PubMed Central PMCID: PMC4891306.

1862

1863 5. Analysis method paper: Lundqvist R, Lilja J, Thomas BA, Lötjönen J, Villemagne VL, Rowe CC, Thurfjell L.
 1864 Implementation and validation of an adaptive template registration method for ¹⁸F flutemetamol imaging
 1865 data. J Nucl Med. 2013 Aug;54(8):1472-8. There are several additional papers that pertain to PiB also, by
 1866 the Klunk/Price group at Pittsburgh.

1867 6. Scanner quality control: Makris NE, Huisman MC, Kinahan PE, Lammertsma AA, Boellaard R. Evaluation
 1868 of strategies towards harmonization of FDG PET/CT studies in multicentre trials: comparison of scanner
 1869 validation phantoms and data analysis procedures. Eur J Nucl Med Mol Imaging. 2013 Oct;40(10):1507-15.

Formatted: Comment Text, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.31" + Indent at: 0.56"

Formatted: Space Before: 6 pt

Formatted: Font: Bold

Formatted: Comment Text, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

Amyloid PET: Quantitative Dynamic Imaging and Methodology

1. Hiroshi Ito, Hitoshi Shimada, Hitoshi Shinotoh, Harumasa Takano, Takeshi Sasaki, Tsuyoshi Nogami, Masayuki Suzuki, Tomohisa Nagashima, Keisuke Takahata, Chie Seki, Fumitoshi Kodaka, Yoko Eguchi, Hironobu Fujiwara, Yasuyuki Kimura, Shigeki Hirano, Yoko Ikoma, Makoto Higuchi, Kazunori Kawamura, Toshimitsu Fukumura, Éva Lindström Böö, Lars Farde and Tetsuya Suhara. Quantitative Analysis of Amyloid Deposition in Alzheimer Disease Using PET and the Radiotracer ¹¹C-AZD2184, Published online: April 14, 2014. *J Nucl Med.*, Doi: 10.2967/jnumed.113.133793

2. Longitudinal Amyloid Imaging Using ¹¹C-PIB: Methodologic Considerations. Bart N.M. van Berckel, Rik Ossenkoppele, Nelleke Tolboom, Maqsood Yaqub, Jessica C. Foster Dingley, Albert D. Windhorst, Philip Scheltens, Adriaan A. Lammertsma, and Ronald Boellaard. *J Nucl Med* 2013; 54:1570–1576, DOI: 10.2967/jnumed.112.113654.

3. Amyloid-B Imaging with Pittsburgh Compound-B and Florbetapir: Comparing Radiotracers and Quantification Methods Susan M. Landau^{1,3}, Christopher Breault³, Abhinav D. Joshi³, Michael Pontecorvo³, Chester A. Mathis⁴, William J. Jagust^{1,2,5}, and Mark A. Mintun³, for the Alzheimer's Disease Neuroimaging Initiative

4. PET Quantification of ¹⁸F-Florbetaben Binding to β -Amyloid Deposits in Human Brains. Georg A. Becker, Masanori Ichise, Henryk Barthel, Julia Luthardt, Marianne Patt, Anita Seese, Marcus Schultze-Mosgau, Beate Rohde, Hermann-Josef Gertz, Cornelia Reininger, and Osama Sabri. *J Nucl Med* 2013; 54:723–731, DOI: 10.2967/jnumed.112.107185.

5. Automated Quantification of ¹⁸F-Flutemetamol PET Activity for Categorizing Scans as Negative or Positive for Brain Amyloid: Concordance with Visual Image Reads. Lennart Thurfjell, Johan Lilja, Roger Lundqvist, Chris Buckley, Adrian Smith, Rik Vandenberghhe and Paul Sherwin. *J Nucl Med* 2014; 55:1623–1629.

6. Accuracy of CT-based attenuation correction in PET/CT bone imaging. M. Abella, A. M. Alessio, D. A. Mankoff, L. R. Macdonald, J. J. Vaquero, M. Desco, and P. E. Kinahan. *Phys. Med. Biol* 2012; 57:9: 2477–2490.

Amyloid PET: Kinetic Modeling (Appendix I)

1. Becker GA, Masanori Ichise, Henryk Barthel, Julia Luthardt, Marianne Patt, Anita Seese, Marcus Schultze-Mosgau, Beate Rohde, Hermann-Josef Gertz, Cornelia Reininger, and Osama Sabri. PET Quantification of ¹⁸F-Florbetaben Binding to β -Amyloid Deposits in Human Brains. *J Nucl Med* 2013; 54:723–731, DOI: 10.2967/jnumed.112.107185.

2. Bullich S, Barthel H, Koglin N, Becker GA, De Santi S, Jovalekic A, Stephens AW, Sabri O. Validation of Non-Invasive Tracer Kinetic Analysis of ¹⁸F-Florbetaben PET Using a Dual Time-Window Acquisition Protocol. *J Nucl Med*. 2017 Nov 24.

3. Carson RE, Channing MA, Blasberg RG, et al. Comparison of bolus and infusion methods for receptor quantitation: application to [¹⁸F]cyclofoxy and positron emission tomography. *J Cereb Blood Flow Metab*. 1993;13:24–42.

4. Cselényi Z, Farde L. Quantification of blood flow-dependent component in estimates of beta-amyloid load obtained using quasi-steady-state standardized uptake value ratio. *J Cereb Blood Flow Metab*. 2015 Sep; 35(9): 1485–1493.

5. Forsberg A, Engler H, Blomquist G, Långström B, Nordberg A. The use of PIB-PET as a dual pathological

Formatted: Font: (Default) Calibri, 12 pt

Formatted: Comment Text, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, Line spacing: single, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5", Tab stops: Not at 4.09"

- and functional biomarker in AD. *Biochim Biophys Acta*. 2012 Mar;1822(3):380-5.
6. Frokjaer VG, Pinborg LH, Madsen J, de Nijs R, Svarer C, Wagner A, Knudsen GM. Evaluation of the Serotonin Transporter Ligand 123I-ADAM for SPECT Studies on Humans. *J Nucl Med*. 2008 Feb;49(2):247-54. doi: 10.2967/jnumed.107.046102. Epub 2008 Jan 16.
7. Giedde A, Aanerud J, Braendgaard, H, Rodell AB. Blood-brain transfer of Pittsburgh compound B in humans. *Front Aging Neurosci*. 2013; 5: 70.
8. Hsiao IT, Huang CC, Hsieh CJ, Hsu WC, Wey SP, Yen TC, Kung MP, Lin KJ. Correlation of early-phase 18F-florbetapir (AV-45/Amyvid) PET images to FDG images: preliminary studies. *Eur J Nucl Med Mol Imaging*. 2012 Apr;39(4):613-20.
9. Lopresti BJ, Klunk WE, Mathis CA, Hoge JA, Ziolkowski SK, Lu X, Meltzer CC, Schimmel K, Tsopelas ND, DeKosky ST, Price JC. Simplified quantification of Pittsburgh Compound B amyloid imaging PET studies: a comparative analysis. *J Nucl Med*. 2005 Dec;46(12):1959-72.
10. Nelissen N, Van Laere K, Thurfjell L, Owenius R, Vandenbulcke M, Koole M, Bormans G, Brooks DJ, Vandenberghe R. J Phase 1 study of the Pittsburgh compound B derivative 18F-flutemetamol in healthy volunteers and patients with probable Alzheimer disease. *Nucl Med*. 2009 Aug;50(8):1251-9.
11. Price JC, Klunk WE, Lopresti BJ, Lu X, Hoge JA, Ziolkowski SK, Holt DP, Meltzer CC, DeKosky ST, Mathis CA. Kinetic modeling of amyloid binding in humans using PET imaging and Pittsburgh Compound-B. *J Cereb Blood Flow Metab*. 2005 Nov;25(11):1528-47.
12. Rostomian AH, Madison C, Rabinovici GD, Jagust WJ. Early 11C-PIB frames and 18F-FDG PET measures are comparable: a study validated in a cohort of AD and FTLD patients. *J Nucl Med*. 2011 Feb;52(2):173-9.
13. Sepulveda-Falla D, Matschke J, Bernreuther C, Hagel C, Puig B, Villegas A, Garcia G, Zea J, Gomez-Mancilla B, Ferrer I, Lopera F, Glatzel M. Deposition of hyperphosphorylated tau in cerebellum of PS1 E280A Alzheimer's disease. *Brain Pathol*. 2011 Jul;21(4):452-63.
14. Sevigny J, Chiao P, Bussière T, Weinreb PH, Williams L, Maier M, Dunstan R, Salloway S, Chen T, Ling Y, O'Gorman J, Qian F, Arastu M, Li M, Chollate S, Brennan MS, Quintero-Monzon O, Scannevin RH, Arnold HM, Engber T, Rhodes K, Ferrero J, Hang Y, Mikulskis A, Grimm J, Hock C, Nitsch RM, Sandrock A. The antibody aducanumab reduces A β plaques in Alzheimer's disease. *Nature*. 2016 Sep 1;537(7618):50-6.
15. Slifstein M. Revisiting an old issue: the discrepancy between tissue ratio-derived binding parameters and kinetic modeling-derived parameters after a bolus of the serotonin transporter radioligand 123I-ADAM. *J Nucl Med*. 2008 Feb;49(2):176-8. doi: 10.2967/jnumed.107.046631.
16. Tolboom N, Yaqub M, Boellaard R, Luurtsema G, Windhorst A, Scheltens P, Lammertsma AA, van Berckel B NM. Test-retest variability of quantitative [11C]PIB studies in Alzheimer's disease. *Eur J Nucl Med Mol Imaging*. 2009 Oct; 36(10): 1629–1638.
17. van Berckel BN, Ossenkuppele R, Tolboom N, Yaqub M, Foster-Dingley JC, Windhorst AD, Scheltens P, Lammertsma AA, Boellaard R. Longitudinal amyloid imaging using 11C-PiB: methodologic considerations. *J Nucl Med*. 2013 Sep;54(9):1570-6.
18. Wong DF, Rosenberg PB, Zhou Y, Kumar A, Raymond V, Ravert HT, Dannals RF, Nandi A, Brasic JR, Ye W, Hilton J, Lyketsos C, Kung HF, Joshi AD, Skovronsky DM, Pontecorvo MJ. In vivo imaging of amyloid deposition in Alzheimer disease using the radioligand 18F-AV-45 (florbetapir [corrected] F 18). *J Nucl*

[Med. 2010 Jun;51\(6\):913-20.](#)

Package Inserts

Note that U.S. prescribing information is listed below for approved tracers. However, this profile is not limited to the U.S. and prescribing information for the relevant country should be consulted for studies outside of the U.S.

1. Amyvid [package insert]. 2012. Available at: <http://pi.lilly.com/us/amyvid-uspi.pdf>. Accessed June 11, 2013.
2. Vizamyl [package insert]. 2013. [updated February 2017](#). Available at: http://www3.gehealthcare.com/en/Products/Categories/~//media/Downloads/us/Product/ProductCategories/Nuclear-Imaging-Agents_Non-Gatekeeper/Vizamyl/GEHealthcare-Vizamyl-Prescribing-Information.pdf. Accessed May 5, 2014. See https://www.accessdata.fda.gov/drugsatfda_docs/label/2017/203137s008lbl.pdf for the full Prescribing Information (PI).
3. Neuraceq [package insert]. [2014](#)[2017](#). Available at: http://www.accessdata.fda.gov/drugsatfda_docs/label/2014/204677s000lbl.pdf. Accessed May 5, 2014.

Additional Papers – protocols or tracers outside of profile guidance

1. Cselenyi Z, Jonhagen ME, Forsberg A, Halldin C, Julin P, Schou M, Johnstrom P, Varnas K, Svensson S, Farde L. Clinical Validation of 18F-AZD4694, an Amyloid-b-Specific PET Radioligand. *J Nucl Med* 2012; 53:415–424, DOI: 10.2967/jnumed.111.094029.
2. Ito H, Shimada H, Shinotoh H, Takano H, Sasaki T, Nogami T, Suzuki M, Nagashima T, Takahata K, Seki C, Kodaka F, Eguchi Y, Fujiwara H, Kimura Y, Hirano S, Ikoma Y, Higuchi M, Kawamura K, Fukumura T, Lindström Böö E, Farde L, Suhara T. Quantitative Analysis of Amyloid Deposition in Alzheimer Disease Using PET and the Radiotracer 11C-AZD2184, Published online: April 14, 2014. *J Nucl Med.*, DOI: 10.2967/jnumed.113.133793
3. Rowe CC, Pejoska S, Mulligan R, Chan G, Fels L, Kusi H, Reininger C, Rohde B, Putz B, Villemagne VL. Test-retest variability of high and low SA [18F] BAY 94-9172 in Alzheimer’s disease and normal ageing. Poster presented at the Society of Nuclear Medicine Meeting, Salt Lake City, UT, 2009.
4. Tolboom N, Yaqub M, Boellaard R, Luurtsema G, Windhorst AD, Scheltens P, Lammertsma AA, van Berckel BNM. Test-retest variability of quantitative [11C] PIB studies in Alzheimer’s disease.
5. Villemagne VL, Pike KE, Chételat G, Ellis KA, Mulligan RS, Bourgeat P, Ackermann U, Jones G, Szoeké C, Salvado O, Martins R, O’Keefe G, Mathis CA, Klunk WE, Ames D, Masters CL, Rowe CC. Longitudinal Assessment of Aβ and Cognition in Aging and Alzheimer Disease. *Ann Neurol*. 2011 January; 69(1): 181–192. doi:10.1002/ana.22248.
6. Villemagne VL, Ong K, Mulligan RS, Holl G, Pejoska S, Jones G, O’Keefe G, Ackerman U, Tochon-Danguy H, Chan JG, Reininger CB, Fels L, Putz B, Rohde B, Masters CL, Rowe CC. Amyloid Imaging with 18F-Florbetaben in Alzheimer Disease and Other Dementias. *J Nucl Med* 2011; 52:1210–1217, DOI: 10.2967/jnumed.111.089730

3. [\[Link\]](#)

Formatted: No bullets or numbering

Formatted: Comment Text, Indent: Left: 0", Hanging: 0.31", Space Before: 6 pt, Numbered + Level: 1 + Numbering Style: 1, 2, 3, ... + Start at: 1 + Alignment: Left + Aligned at: 0.25" + Indent at: 0.5"

Formatted: No bullets or numbering

Formatted: Font: (Default) Times New Roman

1993 Appendices

1994 Appendix A: Acknowledgements and Attributions

1995 This document is proffered by the Radiological Society of North America (RSNA) Quantitative Imaging
 1996 Biomarker Alliance (QIBA) Nuclear Medicine Coordinating Committee. The Amyloid PET Biomarker
 1997 Committee, a subcommittee of the Nuclear Medicine Coordinating Committee, is composed of physicians,
 1998 scientists, engineers and statisticians representing the imaging device manufacturers, image analysis
 1999 software developers, image analysis facilities and laboratories, biopharmaceutical companies, academic
 2000 institutions, government research organizations, professional societies, and regulatory agencies, among
 2001 others. A more detailed description of the QIBA Amyloid-PET Biomarker Committee and its work can be
 2002 found at the following web link: http://qibawiki.rsna.org/index.php/PET_Amyloid_Biomarker_Ctte

2003 The Amyloid PET Biomarker Committee members (in alphabetical order):

QIBA NM PET Amyloid Biomarker Committee Profile Co-Authors:	
Ronald Boellaard, PhD	University of Groning�en (the Netherlands)
Paul E. Kinahan, PhD	University of Washington
Gregory Klein, PhD	F. Hoffmann - La Roche Ltd.
Adriaan A. Lammertsma, PhD	VU University Medical Center
Dawn C. Matthews, MS, MBA	ADM Diagnostics, LLC
Satoshi Minoshima, MD, PhD	University of Utah
Nancy Obuchowski, PhD	Cleveland Clinic Foundation
Eric S. Perlman, MD	Perlman Advisory Group, LLC
Anne M. Smith, PhD	Siemens Medical Solutions USA, Inc.
Jean-Luc Vanderheyden, PhD	JLVMI Consulting LLC
QIBA NM PET Amyloid Biomarker Committee Profile Contributors:	
Keith Allberg	RadQual, LLC
Matjaz Baraga, MD	University Medical Centre Ljubljana
Parviz Behfarin, MD	Plainview Hospital
Orest B. Boyko, MD, PhD	University of Southern California
Andrew J. Buckler, MS	Elucid Bioimaging Inc.
Christopher Buckley, PhD	GE Healthcare
Santiago (Santi) Bullich, PhD	Piramal Imaging (Germany)
Hyo-Min Cho, PhD	Korea Research Institute of Standards and Science
Patricia E. Cole, PhD, MD	Takeda Pharmaceuticals
Jos� Luis Criales Cort�es, MD	Universidad An�huac
Susan M. De Santi, PhD	Piramal
Michael D. Devous, Sr, PhD	Avid Radiopharmaceuticals
Volker Dicken, PhD	Fraunhofer MEVIS (Germany)
Alexander Drzezga, MD	University Hospital Cologne
Edward A. Eikman, MD	Moffitt Cancer Center
Rachid Fahmi, MSc, PhD	Siemens Medical Solutions USA, Inc.
Andrea Ferrero, PhD	Mayo Clinic

P. Thomas Fletcher, PhD	University of Utah, Scientific Computing & Imaging Institute
Norman L. Foster, MD	University of Utah
Anthony Fotenos, MD, PhD (MSTP)	Division of Medical Imaging Products at CDER/FDA
Amy Fowler, MD, PhD	University of Wisconsin, School of Medicine & Public Health
Kirk Frey, MD, PhD	University of Michigan
Jerry Froelich MD	University of Minnesota
Constantine Gatsonis, PhD	Brown University
Alexander Guimaraes, MD, PhD	Oregon Health & Science University
Anurag Gupta, PhD	PAREXEL International
Albert Guvenis, PhD	Institute for Biomedical Engineering, Bogazici University
Jun Hatazawa, MD	Osaka University, Dept. of Nuclear Medicine and Tracer Kinetics
John M. Hoffman, MD	University of Utah
Makoto Hosono, MD, PhD	Kinki University
Masanobu Ibaraki, PhD	Akita Prefectural Hospital Organization,
Hidehiro Iida, DSc, PhD	National Cerebral & Cardiovascular Center (Osaka, Japan)
Edward F. Jackson, PhD	University of Wisconsin, School of Medicine & Public Health
Abhinay D. Joshi, MS	Avid Radiopharmaceuticals / Eli Lilly
Tomohiro Kaneta, MD, PhD	Yokohama City University Graduate School of Medicine
Vasileios K. Katsaros, MD, PhD	University of Athens (Greece)
Tatsuaki Kobayashi, MS	Visionary Imaging Services, Inc.
Robert Koeppe, PhD	University of Michigan
Eun-jung Kong, MD	Yeungnam University Medical Center (Korea)
Arden J. Kwan, MBBS	The Permanente Medical Group (TPMG)
Ben Kwan, MD	Western University, Ontario
Martin A. Lodge, PhD	Johns Hopkins University School of Medicine
Lawrence (Larry) R. MacDonald, PhD	University of Washington
Nobutoku Motomura, PhD	Toshiba
P. David Mozley, MD	Endocyte, Inc.
Mahoto Mugita, BS	Micron, Inc.
Aaron S. Nelson, MD	MIMvista Corp.
Dennis Nelson, PhD	MIMvista Corp.
Yoshihiro Nishiyama, MD	Kagawa University, Faculty of Medicine Dept. of Radiology
Amy Perkins, PhD	Philips
Cornelia B. Reininger, MD, PhD	Navidea Biopharmaceuticals
Haris Sair, MD	Johns Hopkins University
R. Chandrasiri Samaratunga, PhD	University of Cincinnati
Sandra Sanabria, PhD	Genentech
Ramkumar Saptharishi, PhD	Philips
Annette Schmid, PhD	Takeda Pharmaceuticals
Mark E. Schmidt, MD	Janssen Research and Development (Belgium)
Sara Sheikhabaehi, PhD	Johns Hopkins University School of Medicine
Satinder P. Singh, MD	University of Alabama at Birmingham
Charles Smith, MSCS	Numa Inc.

Lilja B. Solnes, MD	University of Maryland
Rohit Sood, MD, PhD	PAREXEL International
Rathan Subramaniam, MD, PhD, MPH	UT Southwestern Medical Center
Daniel C. Sullivan, MD	Duke University
Na Sun, PhD	Yokohama City University Graduate School of Medicine
John J. Sunderland, PhD	University of Iowa
Mitsuaki Tatsumi, MD	Osaka University
Huseyin G. Toré	University of Minnesota
Benjamin M.W. Tsui, PhD	Johns Hopkins University School of Medicine
Lauren Uzdienski, BFA	Technical Writer
Ronald Van Heertum, MD	BioClinica, Inc.
Richard L. Wahl, MD, FACR	Mallinckrodt Institute of Radiology, Washington University
Angela Y. Wang, PhD	The University of Utah
Wolfgang Weber, MD	Memorial Sloan-Kettering Cancer Center
Shuji Yamamoto, PhD	National Cancer Center (Japan)
Brian E. Zimmerman, PhD	National Institute of Standards and Technology (NIST)

The Amyloid PET Biomarker Committee and Nuclear Medicine Coordinating Committee are deeply grateful for the support and technical assistance provided by the staff of the Radiological Society of North America.

Appendix B: Background Information for Claim

A meta-analysis of published data was performed to determine the repeatability of amyloid PET imaging with ¹⁸Fluorine labeled radiotracers. Two types of repeatability studies were considered. The first of these restricted the test-retest period to less than 60 days, over which factors such as longer term scanner drift or appreciable amyloid accumulation would not occur. These studies provided the basis of the wCV value used in the technical performance Claim. The second set of studies compared baseline values to those acquired after a two year period, a typical clinical trial duration. Since amyloid accumulation is unlikely to occur in a majority (though not all) of amyloid negative cognitively normal subjects, longitudinal values in this group were examined. These studies were not used to determine the wCV but did provide a practical indicator of longer term technical variance given a population presumed to be fairly stable with regard to amyloid pathology.

Test-Retest studies: Test-retest amyloid PET studies were identified for the tracers florbetapir (Joshi et al, 2012, scans within 4 weeks) and flutemetamol (Vandenberghe et al, 2010, scans 7 to 13 days apart). Other available studies with images acquired during this time period were excluded for reasons including: a) use of 11C-PIB and a 60 to 90 minute timeframe at the end of a full dynamic scanning session where greater technical variability is observed; this can be due to subject motion and also to low signal whereby decay correction amplifies the noise contribution; and b) intentional varying of administered radioactivity during the study to test the impact of that parameter. The study by Joshi et al acquired florbetapir PET images in 10 AD patients and 10 healthy controls (HC) over a time window of 50 to 70 minutes post injection, and used whole cerebellum as the reference region. Mean Repeatability Coefficient (RC) and 95% confidence

Formatted: Font: Bold

intervals (CI) were 5.38% (3.76% to 9.44%) for AD subjects and 3.32% (2.32% to 5.84%) for HC. Values for wCV were 1.94% and 1.20% respectively. The study by Vandenberghe et al acquired flutemetamol PET images in 5 AD patients over a time period of 85 to 115 minutes post injection, and used cerebellar cortex as the reference region. Mean Repeatability Coefficient (RC) was 3.18% with a 95% CI of 1.99% to 7.81%. The value for wCV was 1.15%. The greatest (“worst”) value of 1.94% from these studies was applied to the Claim. F As noted in the Claim Considerations, the number of short term test-retest studies was a limitation, and for this reason and for practical context, this value was also compared to the wCVs calculated for the longer term studies described below.

Longer term longitudinal variability: Several studies have examined the effects of applying different reference regions or other parameters to amyloid SUVR data acquired over one or two years. Two studies were identified that measured amyloid SUVR in florbetapir PET scans acquired in subjects from the Alzheimer’s Disease Neuroimaging Initiative (ADNI) at baseline and after 2 years. This period is representative of a clinical trial duration. The table below shows the RC means and 95% CI for these studies, using different reference regions. The mean RC in four of the five cases ranged from 3.45% to 4.45%, within the range of 3.18% to 5.38% of the short term test-retest studies described above (Joshi, Vandenberghe). In the Brendel analyses, SUVRs measured using the same subjects but two different reference regions resulted in an RC% of 9.37% that was more than 2x larger when using a whole (full) cerebellum reference as that using white matter as a reference. This was also double the RC% measured by Chen using a different subset of ADNI scans across three different reference regions: pons, cerebellar cortex, and subcortical white matter. These comparisons suggest the following: 1) even over a longitudinal period of 2 years, it is feasible to achieve the wCV identified through the short term test retest studies above; and 2) choice of reference region coupled with analysis methods can materially impact the RC% and wCV, using the same subject scans.

Formatted: Font: Bold

Author	Chen et al 2015	Chen et al 2015	Chen et al 2015	Brendel et al 2015	Brendel et al 2015
Population	CN	CN	CN	CN	CN
Number of subjects	88	88	88	62	62
Amyloid status	Negative	Negative	Negative	Negative	Negative
Time between scans	2 years	2 years	2 years	2 years	2 years
Reference Region	Pons	Cerebellum	White	Full cerebellum	White
RC%	3.45%	4.45%	4.28%	9.37%	3.81%
95% CI - lower	3.01%	3.87%	3.73%	7.97%	3.24%
95% CI - upper	4.05%	5.21%	5.02%	11.36%	4.61%

CN = cognitively normal

Meta-analysis was performed as a groundwork project to determine the repeatability of amyloid PET imaging with ¹¹C-Pittsburgh Compound B (¹¹C-PIB) and ¹⁸F-fluorine labeled radiotracers using the available literature. A total of 7 studies were included in this meta-analysis. Four studies evaluated the test-retest variability of ¹⁸F-fluorine labeled amyloid tracers (Florbetapir, AZD4694, Flutemetamol, Florbetaben). The

2051 test-retest amyloid PET studies were performed between 1 to 4 weeks apart. The pooled %RC for average
2052 cortical SUVR in patients with AD (n=26) was 10.36% (95% CI= 4.76-14.92). The pooled mean %RC for
2053 average cortical SUVR in HCs (n=22) was 10.41 (95% CI= 3.33-20.3). Three studies evaluated the test-retest
2054 variability of ¹¹C-PIB amyloid imaging. The test-retest amyloid PET studies were performed on the same day
2055 and up to 60 days apart. The pooled mean %RC for average cortical SUVR was 15.4% (95% CI= 8.49-20.05).
2056 The pooled mean %RC for average cortical SUVR in HCs (n=16) was 9.38% (95% CI= 7.55-10.92).

2069 **Appendix C: Conventions and Definitions**

2070 ***Convention Used to Represent Profile requirements***

2071 Requirements for adhering to this Profile are presented in tables/boxes as shown in the example below.
 2072 Shaded boxes are intended future requirements, and are not at this time required for adhering to the
 2073 Profile.

2074 Illustrative example:

2075 Parameter Entity/Actor Normative text: Clear boxes are current requirements
 2076 Shaded boxes are intended for future requirements

Phantom tests: transaxial uniformity measurement	Imaging Site	Using ACR, uniform cylinder phantom or equivalent shall obtain an SUV for a large central ROI of 1.0 with an acceptable range of 0.9 to 1.1.
		Using ACR or uniform cylinder phantom or equivalent shall obtain an SUV for a large central ROI of 1.0 with an acceptable range of 0.95 to 1.05.

2077 Items within tables are normative (i.e. required to be conformant with the QIBA Profile). The intent of the
 2078 normative text is to be prescriptive and detailed to facilitate implementation. In general, the intent is to
 2079 specify the final state or output, and not how that is to be achieved.

2080 All other text outside of these tables is considered informative only.

2081 ***Definitions***

3D	Three-dimensional
11C	Carbon-11, an isotope of carbon
18F	Flourine-18, an isotope of fluorine
AB	Amyloid-B
AC	Attenuation Correction. Attenuation is an effect that occurs when photons emitted by the radiotracer inside the body are absorbed by intervening tissue. The result is that structures deep in the body are reconstructed as having falsely low (or even negative) tracer uptake. Contemporary PET/CT scanners estimate attenuation using integrated x-ray CT equipment. While attenuation-corrected images are generally faithful representations of radiotracer distribution, the correction process is itself susceptible to significant artifacts.
Accreditation	Approval by an independent body or group for broad clinical usage (requires ongoing QA/QC) e.g. ACR, IAC, TJC.
AD	Alzheimer’s Disease
ALARA	As Low As Reasonably Achievable
BBB	Blood Brain Barrier
BP_{ND}	Binding Potential. BP _{ND} is the ratio of the density of available receptors to the affinity of the tracer for the receptor, corrected for the free fraction of ligand in the non-displaceable compartment.
CLIA	Clinical Laboratory Improvement Amendments: Accreditation system for establishing quality standards for laboratory testing.
Co-57	Cobalt-57, an isotope of cobalt
Conformance	Meeting the list of requirements described in this document, which are necessary to meet the measurement claims for this QIBA Profile.

CRF	Case Report Form (CRF) is a paper or electronic questionnaire specifically used in clinical trial research. The CRF is used by the sponsor of the clinical trial (or designated CRO etc.) to collect data from each participating site. All data on each patient participating in a clinical trial are held and/or documented in the CRF, including adverse events.
CRO	Contract Research Organization. A commercial or not-for-profit organization designated to perform a centralized and standardized collection, analysis, and/or review of the data generated during a clinical trial. Additional activities which may be performed by an imaging core lab include training and qualification of imaging centers for the specific imaging required in a clinical trial, development of imaging acquisition manuals, development of independent imaging review charters, centralized collection and archiving of images received from study sites, performing pre-specified quality control checks/tests on incoming images and development and implementation of quality assurance processes and procedures to ensure that images submitted are in accord with imaging time points specified in the study protocol and consistent with the quality required to allow the protocol-specified analysis /assessments
Cs-137	Cesium-137, an isotope of Cesium
CSF	Cerebrospinal fluid
CT	X-ray computed tomography (CT) is a medical imaging technique that utilizes X-rays to produce tomographic images of the relative x-ray absorption, which is closely linked to tissue density.
CTDI	Computed tomography dose index
DICOM	Digital Imaging and Communications in Medicine (DICOM) is a set of standards for medical images and related information. It defines formats for medical images that can be exchanged in a manner that preserves the data and quality necessary for clinical use.
DLP	Dose length product
Dose	Can refer to either radiation dose or as a jargon term for 'total radioactivity'. For example, 10 mCi of 18F-FDG is often referred to as a 10 mCi dose.
DRO	Digital Reference Object
DVR	Distribution Volume Ratio
FDG	Fluorodeoxyglucose
FWHM	Full width at half maximum
HIPAA	Health Insurance Portability and Accountability Act
IAC	The Intersocietal Accreditation Commission (IAC) provides accreditation programs for Vascular Testing, Echocardiography, Nuclear/PET, MRI, CT/Dental, Carotid Stenting and Vein Center.
IAEA	International Atomic Energy Agency
IOD	Information Object Definition
kBq	Kilobecquerel
kVp	Peak kilovoltage
LBM	Lean Body Mass is calculated by subtracting body fat weight from total body weight. The Lean body mass (LBM) has been described as an index superior to total body weight for prescribing proper levels of medications and for assessing metabolic disorders.
mAs	Milliamperere-seconds
MBq	Megabequerel. An SI-derived unit of radioactivity defined as 1.0×10^6 decays per second.
MCI	Mild Cognitive Impairment
mCi	millicuries. A non-SI unit of radioactivity, defined as $1 \text{ mCi} = 3.7 \times 10^7$ decays per second. Clinical FDG-PET studies inject (typically) 5 to 15 mCi of 18F-FDG.
mpi	minutes post injection
MRI	Magnetic Resonance Imaging
NA	North America

NTP	Network Time Protocol
PACS	Picture archiving and communication system
PIB	Pittsburgh compound B, a radioactive analog of thioflavin T.
PET	Positron emission tomography (PET) is a tomographic imaging technique that produces an image of the in vivo distribution of a radiotracer, typically FDG.
PET/CT	Positron emission tomography / computed tomography (PET/CT) is a medical imaging system that combines in a single gantry system both Positron Emission Tomography (PET) and an x-ray Computed Tomography (CT) scanners, so that images acquired from both devices can be taken nearly-simultaneously.
PSF	Point Spread Function
PVEc	Partial Volume Effects Correction
QA	Quality Assurance. Proactive definition of the process or procedures for task performance. The maintenance of a desired level of quality in a service or product, esp. by means of attention to every stage of the process of delivery or production.
QC	Quality Control. Specific tests performed to ensure target requirements of a QA program are met. Typically, this is done by testing a sample of the output against the specification.
QIBA	Quantitative Imaging Biomarkers Alliance. The Quantitative Imaging Biomarkers Alliance (QIBA) was organized by RSNA in 2007 to unite researchers, healthcare professionals and industry stakeholders in the advancement of quantitative imaging and the use of biomarkers in clinical trials and practice.
Qualification	Approved by an independent body or group for either general participation in clinical research (ACRIN-CQIE, SNM-CTN others) or for a specific clinical trial (requires ongoing QA/QC). This includes CROs, ACRIN, SNM-CTN, CALGB and other core laboratories.
ROI	Region of interest. A region in an image that is specified in some manner, typically with user-controlled graphical elements that can be either 2D areas or 3D volumes. These elements include, but not limited to, ellipses, ellipsoids, rectangles, rectangular volumes, circles, cylinders, polygons, and free-form shapes. An ROI can also be defined by a segmentation algorithm that operates on the image. Segmentation algorithms include, but are not limited to, fixed-value thresholding, fixed-percentage thresholding, gradient edge detection, and Bayesian methods. With the definition of an ROI, metrics are then calculated for the portion of the image within the ROI. These metrics can include, but are not limited to, mean, maximum, standard deviation, and volume or area. Note that the term ROI can refer to a 2D area on a single image slice or a 3D volume. In some cases, the term ROI is used to refer to 2D area and the term volume of interest (VOI) is used to refer to a 3D volume. In this Profile, the term ROI is used to refer to both 2D areas and 3D volumes as needed.
SUV	Standardized Uptake Value. A measure of relative radiotracer uptake within the body. Typically defined for a time point t as
SUV_{max}	The maximum SUV within the ROI.
SUV_{mean}	The average SUV within the ROI.
SUV_{peak}	The average SUV within a fixed-sized ROI, typically a 1 cm diameter sphere. The spheres location is adjusted such that the average SUV is maximized.
Tc-99m	Technetium-99m, an isotope of technetium
TOF	Time of Flight (TOF) is a PET imaging technique utilizing differential annihilation photon travel times to more accurately localize the in vivo distribution of a radiotracer.
USP	United States Pharmacopeial Convention establishes written and physical (reference) standards for medicines, food ingredients, dietary supplement products and ingredients in the U.S.
VOI	Volume of Interest

2082

2083

Organizations

AAPM	The American Association of Physicists in Medicine is a member society concerned with the topics of medical physics, radiation oncology, imaging physics. The AAPM is a scientific, educational, and professional organization of 8156 medical physicists.
ABNM	American Board of Nuclear Medicine
ABR	The American Board of Radiology
ABSNM	Nuclear Medicine Physics by the American Board of Science in Nuclear Medicine
ACR	The 36,000 members of include radiologists, radiation oncologists, medical physicists, interventional radiologists, nuclear medicine physicians and allied health professionals.
ACRIN	The American College of Radiology Imaging Network (ACRIN) is a program of the American College of Radiology and a National Cancer Institute cooperative group. Focused on cancer-related research in clinical trials.
ANSI	American National Standards Institute
CQIE	The Centers of Quantitative Imaging Excellence (CQIE) program was developed by ACRIN in response to a solicitation for proposals issued in December 2009 by SAIC-Frederick on behalf of the National Cancer Institute (NCI). The primary objective of the CQIE Program is to establish a resource of 'trial ready' sites within the NCI Cancer Centers Program that are capable of conducting clinical trials in which there is an integral molecular and/or functional advanced imaging endpoint.
CRO	Contract Research Organization. A commercial or not-for-profit organization designated to perform a centralized and standardized collection, analysis, and/or review of the data generated during a clinical trial. Additional activities which may be performed by an imaging core lab include training and qualification of imaging centers for the specific imaging required in a clinical trial, development of imaging acquisition manuals, development of independent imaging review charters, centralized collection and archiving of images received from study sites, performing pre-specified quality control checks/tests on incoming images and development and implementation of quality assurance processes and procedures to ensure that images submitted are in accord with imaging time points specified in the study protocol and consistent with the quality required to allow the protocol-specified analysis /assessments
CTN	The Clinical Trials Network (CTN) was formed by SNMMI in 2008 to facilitate the effective use of molecular imaging biomarkers in clinical trials.
EANM	The European Association of Nuclear Medicine (EANM) constitutes the European umbrella organization of nuclear medicine in Europe
EARL	EANM Research Ltd (EARL) was formed by EANM in 2006 to promote multicenter nuclear medicine and research.
ECOG-ACRIN	A National Cancer Institute cooperative group formed from the 2012 merger of the Eastern Cooperative Oncology Group (ECOG) and the American College of Radiology Imaging Network (ACRIN).
EMA	European Medicines Agency is a European Union agency for the evaluation of medicinal products. Roughly parallel to the U.S. Food and Drug Administration (FDA), but without FDA-style centralization.
EU	European Union
FDA	Food and Drug Administration is responsible for protecting and promoting public health in the U.S. through the regulation and supervision of food safety, tobacco products, dietary supplements, prescription and over-the-counter pharmaceutical medications, vaccines, biopharmaceuticals, blood

	transfusions, medical devices, electromagnetic radiation emitting devices, and veterinary products.
HIPAA	Health Insurance Portability and Accountability Act
IAC	The Intersocietal Accreditation Commission (IAC) provides accreditation programs for Vascular Testing, Echocardiography, Nuclear/PET, MRI, CT/Dental, Carotid Stenting and Vein Center.
IAEA	International Atomic Energy Agency
MITA	The Medical Imaging & Technology Alliance is a division NEMA that develops and promotes standards for medical imaging and radiation therapy equipment. These standards are voluntary guidelines that establish commonly accepted methods of design, production, testing and communication for imaging and cancer treatment products.
NEMA	National Electrical Manufacturers Association is a forum for the development of technical standards by electrical equipment manufacturers.
NIST	National Institute of Standards and Technology is a measurement standards laboratory which is a non-regulatory agency of the United States Department of Commerce.
QIBA	Quantitative Imaging Biomarkers Alliance. The Quantitative Imaging Biomarkers Alliance (QIBA) was organized by RSNA in 2007 to unite researchers, healthcare professionals and industry stakeholders in the advancement of quantitative imaging and the use of biomarkers in clinical trials and practice.
RSNA	Radiological Society of North America (RSNA). A professional medical imaging society with more than 47,000 members, including radiologists, radiation oncologists, medical physicists and allied scientists. The RSNA hosts the world's largest annual medical meeting.
SNMMI	Society of Nuclear Medicine and Molecular Imaging (formerly called the Society of Nuclear Medicine (SNM)). A nonprofit scientific and professional organization that promotes the science, technology and practical application of nuclear medicine and molecular imaging. SNMMI represents 18,000 nuclear and molecular imaging professionals worldwide. Members include physicians, technologists, physicists, pharmacists, scientists, laboratory professionals and more
TJC	The Joint Commission (TJC) accredits and certifies health care organizations and programs in the United States.
UPICT	Uniform Protocols for Imaging in Clinical Trials (UPICT). An RSNA-QIBA initiative that seeks to provide a library of annotated protocols that support clinical trials within institutions, cooperative groups, and trials consortia. The UPICT protocols are based on consensus standards that meet a minimum set of criteria to ensure imaging data quality.

2084

2085

Appendix D: Model-specific Instructions and Parameters

The presence of specific product models/versions in the following tables should not be taken to imply that those products are fully in conformance with the QIBA Profile. Conformance with a Profile involves meeting a variety of requirements of which operating by these parameters is just one. To determine if a product (and a specific model/version of that product) is conformant, please refer to the QIBA Conformance Document for that product.

D.1. Image Acquisition Parameters

The following technique tables list acquisition parameter values for specific models/versions that can be expected to produce data meeting the requirements of Section 3.6.4 ('Phantom Imaging').

These technique tables may have been prepared by the submitter of this imaging protocol document, the clinical trial organizer, the vendor of the equipment, and/or some other source. (Consequently, a given model/version may appear in more than one table.) The source is listed at the top of each table.

Sites using models listed here are encouraged to consider using these parameters for both simplicity and consistency. Sites using models not listed here may be able to devise their own acquisition parameters that result in data meeting the requirements of Section 3.6.4 and conform to the considerations in Section 4. In some cases, parameter sets may be available as an electronic file for direct implementation on the imaging platform.

D.2. Quality Assurance Procedures

Examples of recommended quality assurance procedures are shown for specific GE, Philips, and Siemens PET/CT scanners in the tables below.

QIBA Profile Format 20140221

QC procedures and schedules for Philips Gemini TF, V3.3 and V3.4			
Device	QA Procedure	Frequency	
CT	Tube Calibration	Daily	
	Air Calibration	Daily	
	Noise. On head phantom	Daily	
	Noise and Artifacts. On body phantom	Daily	
	Contrast scale and artifacts	Monthly	
	Impulse Response	Advanced test as needed	
	Slice thickness	Advanced test as needed	
PET	Daily PET CT	System Initialization	Daily
		Baseline collection (analog offsets of all photomultiplier channels)	Daily
		PMT gain calibration	Daily
		Energy test and analysis	Daily
		Timing test	Daily
	AutoQC	Emission sinogram collection and analysis	Daily
		Automated System Initialization	Daily, prescheduled to shorten daily QC
	Uniformity check	Automated Baseline collection	Daily, prescheduled to shorten daily QC
			Monthly
	SUV calibration		Every 6 months, after recalibration, when SUV validation shows discrepancy
	SUV validation		Every 2 months, when PM is performed

2107
2108

QA procedures and schedules for GE Discovery ST, STE, Rx and Discovery 600/700 series PET/CT systems				
Device	QA Procedure	Frequency		
Computers	System reboot	Daily or as needed		
CT	CT tube warm up	Daily or after 2 hours of inactivity		
	Air calibrations (fast cals)	Daily		
	Generator calibrations	Daily		
	CT QA phantom	Contrast Scale	Acquire scans daily	
		High Contrast Spatial Resolution	Acquire scans daily	
		Low Contrast Detectability	Acquire scans daily	
		Noise and Uniformity	Acquire scans daily	
		Slice Thickness	Acquire scans daily	
	PET	PET Daily Quality Assurance (DQA)	Laser Light Accuracy	Acquire scans daily
			Full system calibration	Performed after tube replacement or as PM
Coincidence			Daily	
PET coincidence mean			Daily	
PET coincidence variance			Daily	
Singles			Daily	
PET singles mean			Daily	
PET singles variance			Daily	
Deadtime			Daily	
PET mean deadtime			Daily	
Timing		Daily		
PET timing mean		Daily		
Energy		Daily		
PET energy shift		Daily		
PET singles update gain		Weekly		
Clean database	Weekly			
PET 2D normalization	Quarterly (if appropriate for the system)			
PET 2D well counter correction	Quarterly (if appropriate for the system)			
PET 3D normalization and well counter correction	Quarterly			
Establish new DQA baseline	Quarterly			
Ge-68 source pin replacement	Every 18 months			

2109

QIBA Profile Format 20140221

QA procedures and schedules for Siemens Biograph 6/16 Hi-Rez, Biograph 16 Truepoint, Biograph 16 Truepoint with TrueV, PET Syngo 2010A, Biograph mCT

Device	QA Procedure	Frequency	
Computers	Restart computers	Daily at Startup	
	Clear scheduler	Daily	
	Clear network, local, and film queues	Four times daily	
	Archive patient data	Daily	
	System cleanup/defragmentation	Weekly	
CT	CT Checkup/Calibration	Daily, after 60 minutes of full load, within 1 hour of patient scan	
	CT Quality	Water HU	Daily
		Pixel noise	Daily
		Tube voltages	Daily
PET	PET Daily QC	Daily normalization	Daily
		Computation/ verification of the PET calibration factor (ECF)	Daily
		Normalization results display and sinogram inspection	Daily
		System quality report	Daily
		Partial detector setup: generate crystal region maps/energy profiles	Weekly
		Full detector setup and time alignment	Quarterly
		Calculate the Cross Calibration Correction Factor	When Co-68 rhantoms are replaced

QA procedures and schedules for Siemens Biograph 6/16 Hi-Rez, Biograph 16 Truepoint, Biograph 16 Truepoint with TrueV, PET Syngo 2010A, Biograph mCT

Device	QA Procedure	Frequency	
Computers	Restart computers	Daily at Startup	
	Clear scheduler	Daily	
	Clear network, local, and film queues	Four times daily	
	Archive patient data	Daily	
	System cleanup/defragmentation	Weekly	
CT	CT Checkup/Calibration	Daily, after 60 minutes of full load, within 1 hour of patient scan	
	CT Quality	Water HU	Daily
		Pixel noise	Daily
		Tube voltages	Daily
PET	PET Daily QC	Daily normalization	Daily
		Computation/ verification of the PET calibration factor (ECF)	Daily
		Normalization results display and sinogram inspection	Daily
		System quality report	Daily
		Partial detector setup: generate crystal region maps/energy profiles	Weekly
		Full detector setup and time alignment	Quarterly
		Calculate the Cross Calibration Correction Factor	When Co-68 rhantoms are replaced

Appendix E: Data fields to be recorded in the Common Data Format

Mechanism

The list below comprises meta-information (i.e. in addition to image values of kBq/ml) that is necessary for quantitatively accurate (i.e. known and minimal uncertainties) of PET SUVs. The intent here is to list what information should be captured rather than the mechanism itself. The format and corresponding mechanism of data capture/presentation is currently unspecified, but ranges from paper notes, to scanned forms or electronic data records, to direct entry from the measurement equipment (i.e. the PET/CT scanner or auxiliary measurement devices such as the radionuclide calibrator) into pre-specified DICOM fields. Ideally all the specified meta-data will be captured by direct electronic entry to DICOM fields, after suitable modification of the DICOM format for PET imaging.

The concept endorsed here is that the needed meta-data is identified. Through revisions of this Profile, the DICOM standard, and technology the meta-data is inserted into the analysis stream (Figure 3) in a more direct manner and technology and accepted standards evolve.

- The needed information, where feasible, is listed in order from least frequently changing to most frequently changing.
- In all cases note whether measurements are made directly or estimated. If the latter case, note the source of information and the date and time (e.g. if subject cannot be moved from bed to measure weight or height).

Data fields to be recorded:

1. Site specific
 - a. Site information (include name and/or other identifiers)
 - b. Scanner make and model
 - c. Hardware Version numbers
 - d. Software Version numbers
 - e. Confirmation that scanner used was previously qualified (or not)
2. Protocol specific
 - a. PET
 - i. Duration per bed
 - ii. Acquisition mode (3D)
 - iii. Reconstruction method
 - b. CT technique (if PET/CT scan)
3. Scanner specific QA/QC
 - a. Most recent calibration factors (scanner)
 - b. Scanner daily check values
 - c. most recent clock check
 - d. most recent scanner QA/QC
4. Subject exam specific
 - a. Weight (optional)
 - b. Pre- and post-injection assayed activities and times of assay
 - c. Injection time
 - d. Site of injection (and assessment of infiltration)
 - e. Net injected activity (calculated including decay correction)
 - f. Uptake time

2156

2157

2158

Appendix F: Testing PET Display and Analysis Systems with the UW-PET QIBA Amyloid Digital Reference Object (DRO) Series

2159

2160

2161

2162

2163

2164

2165

The University of Washington-PET QIBA PET Amyloid DRO series is a synthetically generated set of DICOM image files of known voxel values for PET. The PET data were derived from a single subject's MRI scan (provided with the DRO series). The UW-PET QIBA DRO series is intended to test the computation of standardized uptake value ratios (SUVRs) by PET amyloid image analysis workstations (IAWs). This is motivated by vendor-specific variations in PET amyloid IAWs. The development of the UW-PET QIBA DRO series is supported by the Quantitative Imaging Biomarker Alliance (QIBA) and the University of Washington.

2166

2167

2168

2169

2170


The primary goals and objectives of the UW-PET QIBA DRO series are to support the QIBA PET amyloid 'Performance Assessment: Image Analysis Workstation and Software' efforts for Profile development. This will be done by (1) visual evaluation of the target and reference region placement, (2) evaluation and validation of SUVR calculations with regards to reproducibility and linearity and (3) providing a common reference standard that can be adopted and modified by IAW manufacturers.

2171

2172

2173

As mentioned above, the UW-PET QIBA PET Amyloid DRO series is based on a single segmented MRI scan of a patient. The MRI scan digitally had the skull and skin removed, and then was segmented into GM, WM, and CSF, which allows for different values of PET activity to be simulated in these regions.

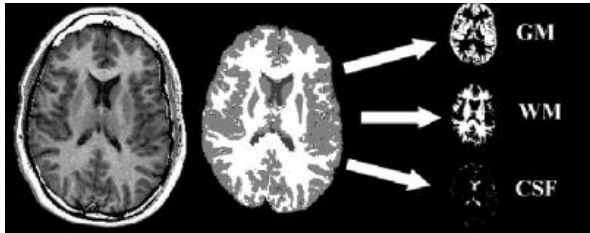

2174

2175

2176

Illustration of how the DRO series was created.

2177

2178

2179

2180

Normally, a system of measurement would have assessments and conformance levels for bias, linearity and reproducibility. Since the claim in this Profile is a longitudinal claim (as opposed to a cross-sectional claim) and the same imaging methods shall be used at each time point, bias does not need to be assessed. Therefore, conformance assessment as detailed here will focus on linearity and reproducibility.

2181

Linearity

2182

2183

2184

The linearity of the IAW will be assessed by testing a range of different subjects, as defined by varying SUVR values. The table below gives more detail about the simulated subjects and their respective SUVR values. The activity in the CSF region will be set to 0.

Subject	GM Activity	WM Activity	GM/WM Ratio
1	0.9X	X	0.9
2	1.0X	X	1.0

3	1.1X	X	1.1
4	1.2X	X	1.2
5	1.3X	X	1.3
6	1.4X	X	1.4

2185

2186 Therefore, 6 subjects were simulated in the DRO series which will be later used to test the linearity of the
2187 IAW.

2188 **Reproducibility**

2189 The reproducibility of the IAW will be assessed by making multiple realizations of the same subject. This
2190 can be thought of as simulating test-retest multiple times on the same subject. The multiple realizations
2191 will be done by adding typical levels of clinical noise five times to each subject. Please see the figure below
2192 for a pictorial representation.

2193 **The DRO Series**

2194 The simulation of six subjects and five realizations means that the DRO series will contain 30 simulated PET
2195 volumes. These volumes will be stored in DICOM format and can be downloaded from the Quantitative
2196 Imaging Data Warehouse (QIDW), with the link given below.


2197 **IAW Conformance Procedure**

- 2198 a. Download the UW-PET QIBA PET Amyloid DRO series from QIDW [<give link when ready>](#).
- 2199 b. Analyze the 30 volumes using the same procedure, target regions and reference regions as will be
2200 used with patient data.
- 2201 c. For each target region for a fixed reference region, the information to form the graph below should
2202 be calculated, and will be called a given target's results, e.g. (Frontal Target/Whole Cerebellum
2203 Reference Region) Results:

Example Output – For Single Target Region

Will be one graph for each Target Region if single reference region is used
 If multiple reference regions, then total graphs = (number of target regions) x (number of reference regions)

IAW Conformance – Target Region 1

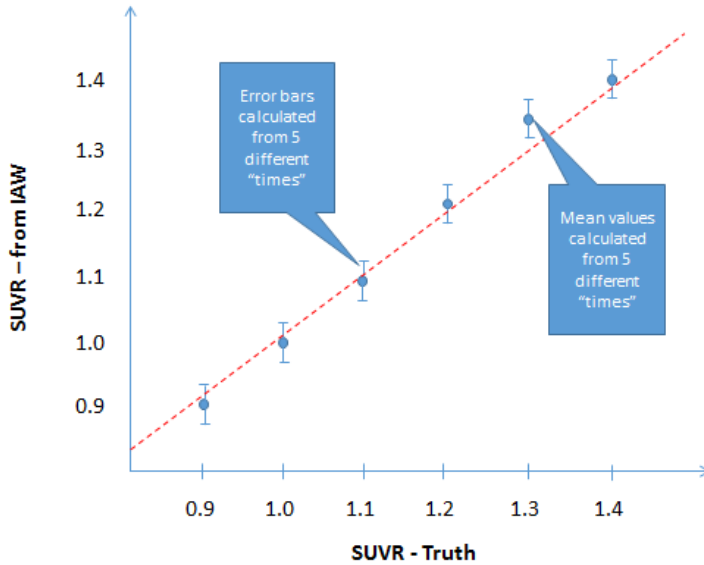

2204

2205

2206

2207

2208

2209

2210

2211

2212

2213

2214

2215

2216

2217

2218

2219

2220

4. If multiple reference regions will be used, generate the same information as in point 3 above using this new reference region. The final number of target results or graphs will be (number of target regions) x (number of reference regions).
5. The following statistical analysis should be performed on each target result.
 - a. Fit an ordinary least squares (OLS) regression of the Y_i 's on X_i 's (where Y 's are the SUV measurements from the IAW, and X 's are the true SUV measurements). A quadratic term is first included in the model: $Y = \theta_0 + \theta_1 X + \theta_2 X^2$.
 - The estimate of θ_0 , θ_1 and θ_2 , along with their 95% Confidence Intervals (CIs), shall be reported as part of the assessment record (see last point below).
 - b. Re-fit a linear model: $Y = A_0 + A_1 X$ (red dotted line on graph above).
 - The estimate of A_0 and A_1 , along with their 95% CIs, shall be reported as part of the assessment record (see last point below).
 - R-squared (R^2) shall be >0.90 for the IAW to be compliant for the given target and reference regions.
 - c. For each of the 6 true SUVR values, calculate the mean (blue points in graph above) of the 5 measurements and the wSD (blue error bars in graph above) using the following equations

where the summations are from J=1 to J=5:

$$\bar{Y}_i = \sum(Y_{ij})/J \text{ and } wSD_i^2 = \sum(Y_{ij} - \bar{Y}_i)^2 / (J - 1).$$

d. Estimate wCV using the equation, where N=6:

$$wCV = \sqrt{\sum_{i=1}^N (wSD_i^2 / \bar{Y}_i^2) / N}.$$

f. Estimate the % Repeatability Coefficient (%RC) using the equation:

$$\%RC = 2.77 \times wCV \times 100.$$

- The %wCV shall be $\leq 2.6\%$ for the IAW to be compliant for the given target and reference regions. (Note that this conformance criterion allows 95% confidence that the %RC of the IAW meets the Profile claim.)
- For future reference, the number of subjects and tests per subjects can be changed in the DRO series, which will change the wCV% threshold as per the table below.

# of Subjects (SUVRs)	# of Realizations (Tests per subject)	wCV% Threshold
6	5	2.6%
7	5	2.8%
9	5	2.9%
11	5	3.0%
6	10	3.1%

6. For each target's results, report the following in a format similar to the example table below.

Ref Region	Visual Placement Check	Target Region	Visual Placement Check	θ_0	θ_1	θ_2	A_0	A_1	R^2	$R^2 > 0.90$	wCV	%RC	%RC $\leq 2.6\%$
1	Pass	1	Pass	0.03	0.91	0.01	0.1	0.97	0.92	Pass	7.6×10^{-3}	2.1	Pass
1	Pass	2	Pass	0.05	0.9	0.02	0.07	0.95	0.91	Pass	1.05×10^{-2}	2.9	Fail
1	Pass	3	Fail	-	-	-	-	-	-	-	-	-	-
1	Pass	4	Pass	0.16	0.81	0.14	0.14	1.2	0.85	Fail	-	-	-
2	Fail	-	-	-	-	-	-	-	-	-	-	-	-
3	Pass	1	Pass	0.03	0.91	0.01	0.1	0.97	0.92	Pass	7.6×10^{-3}	2.1	Pass
3	Pass	2	Pass	0.04	0.95	0.04	0.03	0.92	0.93	Pass	8.0×10^{-3}	2.2	Pass
...

The table report above should be saved and archived with any PET amyloid patient study that is compliant

2240 with this Profile.

2241

Appendix G: Best Practice Guidance for the Hoffman Brain Phantom

- Make sure that before the 18-F or 18-FDG is added, you start with a completely filled phantom (less ~100ml, described later). It is helpful to fill the phantom with water the day before to help remove small air bubbles.
- Purified or distilled water is preferred, normal tap water is OK.
- When you are filling, it helps to tip the phantom slightly (use a syringe or similar object underneath one side). It also helps to open more than one of the filling ports while filling. Once you have the phantom completely filled, then use a 50-60cc syringe to take out ~75-100ml before injecting with the FDG. This allows for better mixing.
- Prepare the F18 tracer (typically FDG) in a volume of **3-5ml**, calibrated for an injected amount of 0.5-0.6 mCi (18.5 – 22.2 MBq) at the projected time of scanning.

Formatted: Justified


Formatted: Justified, Indent: Left: 0.25", No bullets or numbering



- Switch the needle on the syringe to a long, blunt tip needle. Insert through the top filling port (the brain's **anterior** side) until the tip of the needle is **approximately half way down through the phantom**. Rinse the syringe 2 or 3 times to reduce the residual in the syringe.
- To ensure there is no tracer left in the original (short) needle, attach that needle, and also rinse 2-3 times.
- Measure the residual in both needles and syringe. We suggest you place these in a surgical glove before placing in the dose calibrator to prevent contamination of the dose calibrator.

- Once injected, replace the cap and roll back and forth vigorously for about 5min. Occasionally, pick up and tip up and down the other way.
- Top off as best you can, filling through 1 or two of the ports (wherever bubbles are).
- Roll a 2nd time, briefly for about 1min. this will help to get bubbles out.
- Top off a 2nd time. The focus now is to remove any remaining air getting bubbles. An effective method is to hold upright (with filling ports up), and shake back and forth vigorously to make the bubbles rise. (Remember when filling to minimize spills. Wipe with a paper towel, and this goes to radioactive waste)
- Roll a final 3rd time. Then top off again to remove any remaining air bubbles.
- As a final check, look through the phantom at a bright light to check for bubbles. If there are some large bubbles (greater than ~3 mm), try another shaking/tapping/rolling/filling session.
- Finally, if you do the CT scan and notice there are big bubbles or air spaces, take the phantom and try to top off/remove the bubbles before doing the finally CT/Pet scans

Generally, this process takes about 10-20min.

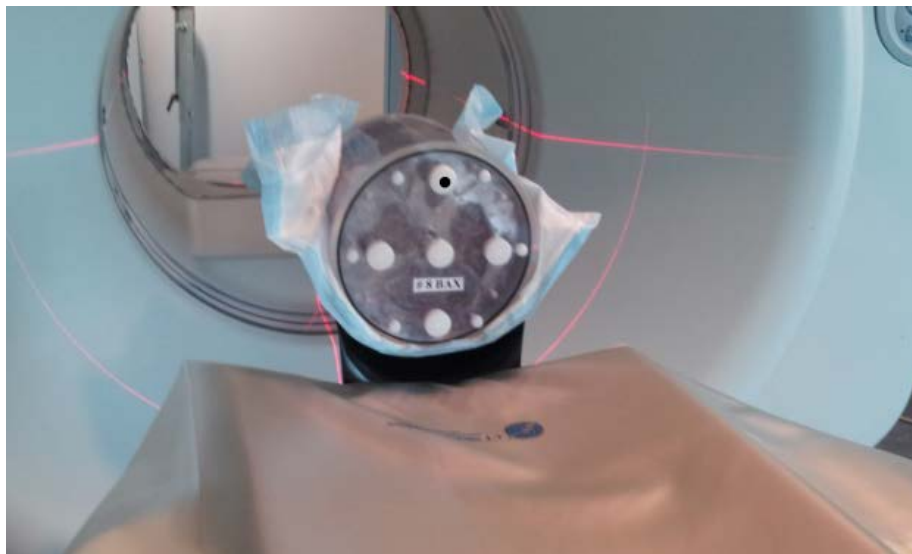

Position the phantom on the scanner bed with the filling ports towards the foot of the bed, and the anterior filling port at 12 o'clock. (In this position, the cerebellar lobes should be visible at the bottom of the phantom, and should appear in the reconstructed image as if you were imaging a supine subject).

Formatted: Justified

Appendix H: Detailed Example of Hoffman Phantom Data Analysis

Formatted: English (United States)

Appendix H: Detailed Example of Hoffman Phantom Data Analysis

Formatted: Justified

The basic methodology in the quantitative analysis is to first align the test scan to the digital atlas using an affine registration, then to intensity normalize the data, and finally to find a smoothing factor for the digital atlas that best matches the spatial resolution of the test scan. Once a registered, the intensity normalized test image and smoothed gold standard are computed, and the difference image can be viewed visually and quantified by various methods described below to assess overall scan quality.

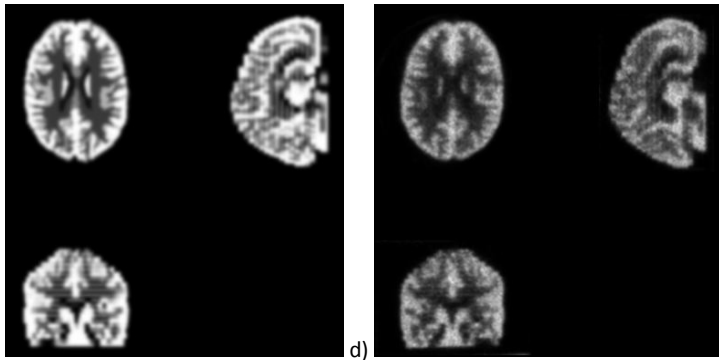
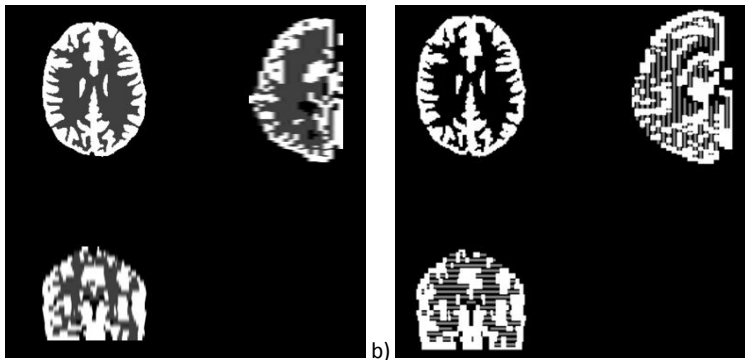


Figure 1. Digital Hoffman Phantom. a) 19-slice version supplied by Data Spectrum. b) 90-slice version modeling more accurately individual layers of each slice. c) smoothed version of the 90-slice digital phantom. d) sample real phantom data obtained from the high-resolution HRRT scanner.

Phantom Description

Phantom Description

The interior of the Hoffman brain phantom is composed of 19 separate plexiglass plates, each 6.1 mm thick. To achieve the 4:1 gray:white uptake ratio via displacement of a uniform concentration of radioisotope

Formatted: Justified, Space After: 0 pt

2302 solution, each plate is composed of a “sandwich” of eight separate layers, of “gray” slices (G), cut to the
2303 shape of modeled gray matter, and “white” slices (W), cut to the shape of modeled white matter. Areas of
2304 CSF are left completely void. Each layer is therefore composed of a “sandwich” in this order:
2305 GG|W|GG|W|GG. The most caudal slice and most cranial slice consist of just 4 gray layers (GG|GG).

2306
2307 Data Spectrum, who manufactures the phantom, supplies a 256x256x19 voxel digital atlas that models the
2308 phantom appearance as having one of 3 types of uniform areas in each 6.1 mm slice (gray=4, white=1,
2309 csf=0). See Figure 1a. Dr. Bob Koeppel from the University of Michigan, in collaboration with Data Spectrum
2310 and CTI (now Siemens) constructed a more accurate 160x160x90 voxel, 1.548x1.548x1.548 mm version of
2311 this phantom that models the individual layers between the slices. Each slice of this 90-slice phantom
2312 represents either a “GG” all gray layer with values either 0 or 1.0; or a “GW” layer with values either 0, 0.5
2313 or 1.0. This digital phantom (Fig 1b,c) looks much more like data obtained from a high-resolution PET
2314 scanner (Fig 1d), and can be smoothed to approximate images from lower-resolution scanners. The
2315 individual layers can actually be seen in some higher resolution scanners, such as the Siemens HRRT.

2316
2317
2318 One important item to note is that the actual phantom size, especially the actual physical slice thickness of
2319 each phantom, can vary slightly. Therefore, when comparing data, it is important to deal with the scaling
2320 appropriately. Alternatively, if comparisons are made between two acquisitions, one must insure that the
2321 identical phantom is used in the comparison. If there are multiple phantoms in use, it is good practice to
2322 track each phantom with an appropriate identification number.

2323
2324 Regarding smoothing, it is assumed that the PET scanner resolution can be modeled by smoothing with a
2325 Gaussian kernel with the same size in the transaxial direction (i.e. x and y direction), and another size in the
2326 axial direction (i.e. z direction). This is approximate, since blurring increases transaxially away from the
2327 center, and is different in the radial and tangential directions. Also, axial resolution is degraded in the outer
2328 end planes of the scanner. However, the uniform smoothing assumption is fairly reasonable for head
2329 imaging, where the field of view is fairly close to the center of the scanner.

2330 Methods and Metrics

2331 **Methods and Metrics**

2332 **Method Overview**

2333 The method for quantitative analysis can be summarized by the following steps:

- 2334 1) Sum a dynamic PET test image, which we will call the “Source Image” acquisition, to produce a
2335 single average PET volume
- 2336 2) Register the averaged Source Image to the 90-slice digital reference using an affine transformation
- 2337 3) Determine Gaussian smoothing factors FWHM_{xy}, FWHM_z, to be applied to the digital phantom so
2338 that it best matches the registered Source dataset.
- 2339 4) Compute image metrics on differences between the matched smooth “gold standard” data, and the
2340 registered Source data.
- 2341 5) Create different images and graphics to augment a visual assessment of image quality.

2342 **Relevant Data Files**

2343 The following input and reference files are used in the analysis:

2344 Reference Files

2345 **ctiHoffman0.0_0.0.nii** – This is the 160x160x90 digital gold standard data.


2346 **ctiHoffman5.0_5.0.nii** – This is ctiHoffman0.0_0.0.nii smoothed by a Gaussian kernel 5.0 mm FWHM in the
 2347 x, y, and z dimensions. This represents an image at about the resolution of the highest-resolution scanners,
 2348 such as the HRRT.

2349 **HoffmanVOI5mm6Level.25_95BrainMask.nii** – This is a volume-of-interest (VOI) mask file with six levels
 2350 created in PMOD using multi-level thresholding on the smoothed, phantom file, **ctiHoffman5.0_5.0.nii**. The
 2351 resulting segmentation is seen in Figure 2. Idealized voxel intensities for CSF, white matter and gray matter
 2352 are 0.0, .025, 1.0 respectively, but blurring of the digital phantom results in a partial volume effect so that
 2353 voxel values vary continually between 0.0 – 1.0. Regions were defined with the following IDs and
 2354 thresholding criteria as follows:

Region ID	Threshold	Description
1	Val < 0.01 outside brain contour	nonbrain
2	Val < 0.05	Pure CSF
3	0.05 < Val < .20	White/CSF mixture
4	0.20 < Val < .30	Mostly “pure” white
5	.30 < Val < .90	Gray/white mixture
6	.90 < Val	Mostly “pure” gray

2355 Regions 4 and 6, which represent areas of mostly white and gray matter, respectively, are the main regions
 2356 used for comparison in the analysis.

2357

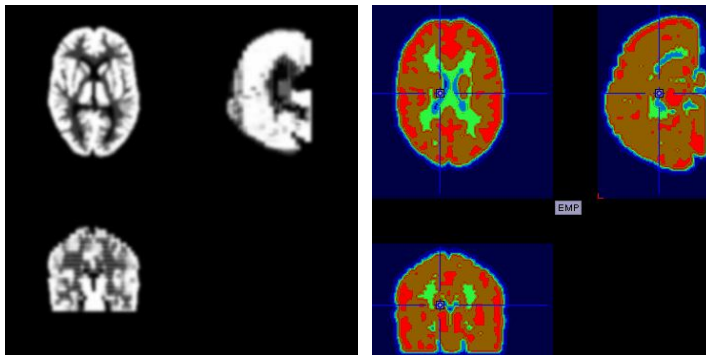

2358

2359 Figure 2. Six-region Volume of Interest mask. The smoothed digital reference (left), and the volume of
 2360 interest mask volume created in PMOD using multi-thresholding segmentation (right). The VOI mask is used
 2361 to define areas representing primarily pure gray (shown in red) and pure white matter (shown in green).
 2362 These regions are used for image intensity normalization and various image quality metrics.

Formatted: Justified

Formatted: Justified

2353
2354
2355
2356
2357
2358
2359
2370
2371
2372
2373
2374
2375
2376
2377
2378
2379
2380
2381
2382
2383
2384
2385
2386
2387
2388
2389
2390
2391
2392
2393
2394
2395
2396
2397
2398

Input files

SourceXXX – original dynamic PET data. Usually in DICOM format, and for this profile is recommended to be a 4 x 5 minute acquisition.

Intermediate Files

Avg **SourceXXX.nii** – summed dynamic data.

RegSourceXXX.nii – summed dynamic data registered to 160x160x90 voxel digital phantom template

RegSourceNorm.nii – version of **RegSourceXXX.nii** intensity normalized to values between 0 and 1.0.

Output Files

Volumes

RegSourceXXXFit.nii – smoothed version of the Hoffman digital template , **ctiHoffman0.0_0.0.nii** , that is the best fit to **RegSourceNorm.nii**.

RegSourceXXXAbsDiff.nii – absolute difference volume between RegSourceXXXFit.nii and RegSourceNorm.nii

Text

RegSourceXXXfit.txt – summary output file

JPG -

RegSourceXXXXplotAbsDiffProfile.jpg – plot showing slices-by-slice profiles of ROI absolute difference sums vs image plane number in the RegSourceXXXAbsDiff.nii volume for these four ROIs: whole volume, whole brain, pure grey ROI, pure white ROI (see example plot <>)

RegSourceXXXXplotGrayWhiteProfile.jpg - plot showing slice-by-slice profiles of ROI # 4 (pure white matter) and #6 (pure grey matter)" ratios between the reference data (RegSourceXXXFit.nii) and the test data (RegSourceNorm.nii) (see example plot <>)

RegSourceXXXXplotImgDiff.jpg - central three orthogonal planes through **RegSourceXXXAbsDiff.nii**, gray scale set between -0.2 and 0.2.

RegSourceXXXXplotImgNorm.jpg – central three orthogonal planes through **RegSourceNorm.nii**, gray scale set between 0.0 and 1.0

Method Details: Processing Steps

Method Details—Processing Steps

Formatted: Justified, Space After: 0 pt

Formatted: Justified, Space Before: 6 pt, After: 0 pt

Formatted: Space After: 0 pt

Formatted: Space Before: 6 pt, After: 0 pt

Formatted: Justified

Formatted: Font: Not Bold

Formatted: Font: Not Bold

Formatted: Normal, Left

Formatted: Justified

- 2399 1) Manual step: Load/visual check of image data. Add to PMOD batch file list
2400 Images need to be manually loaded to check visually that the orientation is correct. If the image loads
2401 using default parameters, it can be simply added to a PMOD file list for later batch processing. If the
2402 default settings do not work, the image must be manually loaded using the correct image reorientation
2403 switches, saved as a new dynamic file, then added to the PMOD batch file list.
- 2404 2) Batch step: PMOD script: Dynamic Averaging, Affine Registration to Hoffman Digital reference
2405 This step sums the dynamic PET data to obtain an averaged PET source file, and then registers the
2406 averaged PET to the Hoffman reference image. It is assumed that there is no motion between image
2407 time frames, so a motion correction step is not necessary like it would be for a patient study. As a
2408 reference image, the version of the Hoffman reference smoothed with a 5 mm isotropic Gaussian filter
2409 is used (**ctiHoffman5.0_5.0.nii**). This represents the resolution of an image that would be expected from
2410 the highest resolution PET scanners. In PMOD's registration module, Normalized Mutual Information
2411 and the "scale" option are selected to allow an affine match that will compensate for slightly different
2412 phantom actual sizes. No other pre-smoothing is used during the registration. The batch process saves
2413 the averaged and the registered dataset as two separate files. This step can be run on one or many
2414 different PET files. PMOD is not set up yet to record the reorientation matrix (I have requested this), so
2415 we do not have a full track of all operations.
- 2416 3) Batch step: Matlab script: Normalize PET, Fit Smoothing Model, Quantify Difference Image
2417 Once the PET source has been registered to the Hoffman reference, the following steps are carried out
2418 using a matlab script:
- 2419 a) *Normalize the Registered PET source intensity.* The noiseless digital phantom has values ranging
2420 between 0.0 and 1.0. Rather than normalizing to maximum intensity of the source image, the
2421 following approach is taken which adjusts for the partial volume effect and for the expected
2422 Poisson-related variability around the mean for the expected values in the areas representing
2423 gray and white matter. Using the 6-level VOI mask, we use region 6, the area representing mostly
2424 pure gray matter, as a reference region. The mean intensity of voxel values in this region is
2425 computed in both the smoothed reference volume and the registered source volume. A scale
2426 term is computed as the ratio of reference volume gray region mean intensity / source volume
2427 gray region mean intensity. This results in the mean with the area representing pure gray area to
2428 be set to a voxel intensity of 1.0 in the normalized image.
- 2429 b) *Fit Gaussian smoothing kernels, FWHM_{xy} and FWHM_z.* An unconstrained nonlinear estimation
2430 approach is used to find the Gaussian smoothing kernels that produce a smoothed version of the
2431 digital reference phantom best matching the normalized source volume. (using Matlab's
2432 "fminsearch" function). We investigated various image difference measures: absolute difference,
2433 squared difference, correlation, and brain-masked differences, and the simple absolute
2434 difference appeared to work well. The code is written so that any of these options can be
2435 selected, but the default is the absolute difference.
- 2436 2) Calculation of Quality Metrics from the Normalized Source Image and Difference Image
2437 The difference between the normalized source image and the digital reference smoothed to fit the
2438 source image is the main basis for the comparison. Additionally, some measures can also be computed
2439 from the normalized source image alone. Basic ideas to consider in this analysis include:
- 2440 - The ideal gray:white contrast ratio should be 4:1 in a noise free setting with perfect spatial
2441 resolution. We need to consider the partial volume effect, so most evaluations are made in
2442 comparison to global or VOI measures on the noise-free smoothed digital reference.

- 2443 - For evaluations using a uniform phantom, the usual figure of merit for an acceptable measurement
2444 variance is +/- 10% from the mean both in-plane and axially. Therefore, an absolute difference of
2445 about 10%, i.e. +/- 0.1 intensity units would ideally be a maximum difference between the
2446 normalized source and the smoothed reference image.

Quality Metrics

a) *Global Volume Metrics*

- 2448 i) **Comparison of fit smoothing parameters to published data from ADNI / Bob Koeppe's group.**
2449 This value should be consistent for a given scanner type. Differences in Z-smoothing compared
2450 to ADNI results are expected due primarily to Z-scaling during the affine registration process.
2451 Based on empirical observation, there most likely is a problem if the fit smoothing parameters
2452 differ by more than 1 mm FWHM.
- 2453 ii) **Average Global Absolute Difference – total image volume** : ideally, this should be less than
2454 10%, therefore less than 0.1 for the images intensity normalized to values between 0.0 and 1.0.
- 2455 iii) **Average Global Absolute Difference in the brain region only**: ideally, this should be less than
2456 10%, therefore less than 0.1 for the images intensity normalized to values between 0.0 and 1.0.
- 2457 iv) **Gray:White mater ratio in the source image**. Ideally, this should be 4.0. For scanners of lower
2458 resolution we would expect the value to be less.
- 2459 v) **Ratio of Gray:White in the Source image compared to smoothed reference**. Ideally, this should
2460 be 1.0. Would expect at most a 10% variation.
- 2461 vi) **Ratio of White matter intensity standard deviation in the Source imaging compared to the
2462 smoothed reference**: This measure gives an indication of image noise. By comparing to the
2463 reference volume, variation with the white matter region due to the partial volume effect
2464 should cancel out.
- 2465 vii) **Ratio of Gray matter intensity standard deviation in the Source imaging compared to the
2466 smoothed reference**. : This measure gives an indication of image noise. By comparing to the
2467 reference volume, variation with the white matter region due to the partial volume effect
2468 should cancel out.
- 2469 b) *Slice-by-slice Metrics (computed between planes 10-80, which represent the plane with brain data in
2470 the Hoffman reference volume)*
- 2471 i) **Average Slice Absolute Difference – total slice**: ideally, this should be less than 10%, therefore
2472 less than 0.1 for the images intensity normalized to values between 0.0 and 1.0.
- 2473 ii) **Average Slice Absolute Difference – brain region only**: ideally, this should be less than 10%,
2474 therefore less than 0.1 for the images intensity normalized to values between 0.0 and 1.0.
- 2475 iii) **Average Slice Absolute Difference – gray matter only (VOI region #6)**: ideally, this should be
2476 less than 10%, therefore less than 0.1 for the images intensity normalized to values between 0.0
2477 and 1.0.
- 2478 iv) **Average Slice Absolute Difference – white matter only (VOI region #4)**: ideally, this should be
2479 less than 10%, therefore less than 0.1 for the images intensity normalized to values between 0.0
2480 and 1.0.
- 2481 v) **Ratio of mean gray intensity in VOI region #6 for Source compared to smoothed reference**:
2482 ideally, this should be 1.0
- 2483 vi) **Ratio of mean white intensity in VOI region #6 for Source compared to smoothed reference**.
2484 Ideally, this should be 1.0.
- 2485 vii) **Profile Coefficient of Variation for Gray slice mean gray intensity**. This metric can be used as a
2486 sentinel for unacceptable variations in axial sensitivities.
2487
2488

3) Outputs: Graphics, Text Summary and Imaging volumes

- a) JPGs
 - i) 3 orthogonal slices through the center of the difference volume – color bars set to +/- 0.2 for all evaluations to highlight significant areas that differ from the reference volume. A
 - ii) 3 orthogonal slices through the normalized, registered source volume
 - iii) Slice-by-slice profiles of error measures between source and reference volumes
 - iv) Slice-by-slice profiles of the ratio of mean gray and white matter region intensity regions for the source volume compared to the reference volume.
- b) Text file
 - i) Numerical values for the global and plane-by-plane metrics
- c) Image volumes
 - i) Difference Volume
 - ii) Fit Smoothed Reference Volume

Note: Matlab Modules Used. In addition to the base Matlab package, the processing pipeline used the standard Matlab Image Processing Toolbox and the Optimization Toolbox. The pipeline also used the 3rd party Matlab package for reading, writing and displaying NIFTI files, “Tools for NifTI and ANALYZE image”, found at <http://www.rotman-baycrest.on.ca/~jimmy/NIFTI>.


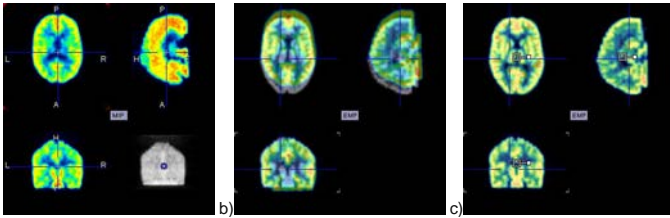



Figure 3. Affine Registration Process. Source image in original orientation (a). Source image (colored grayscale, and digital gold standard (grayscale) unregistered (b), and after registration in PMOD (c).

Example Results using the ADNI Hoffman Qualification Data


Example 1. Good quality scan. Siemens HIREZ (037_P_0001)

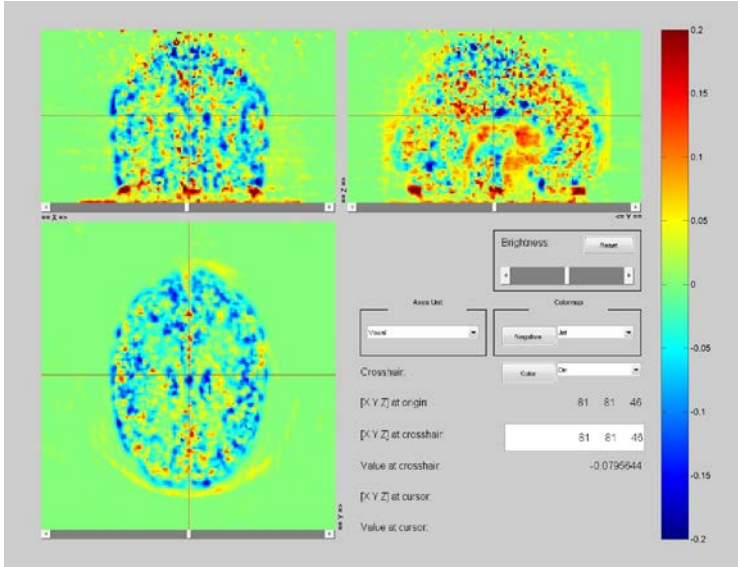


2514
2515

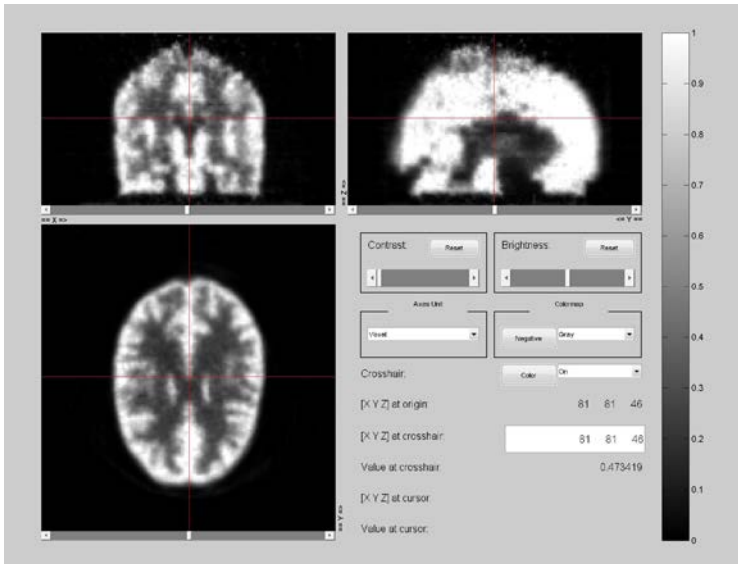

2516

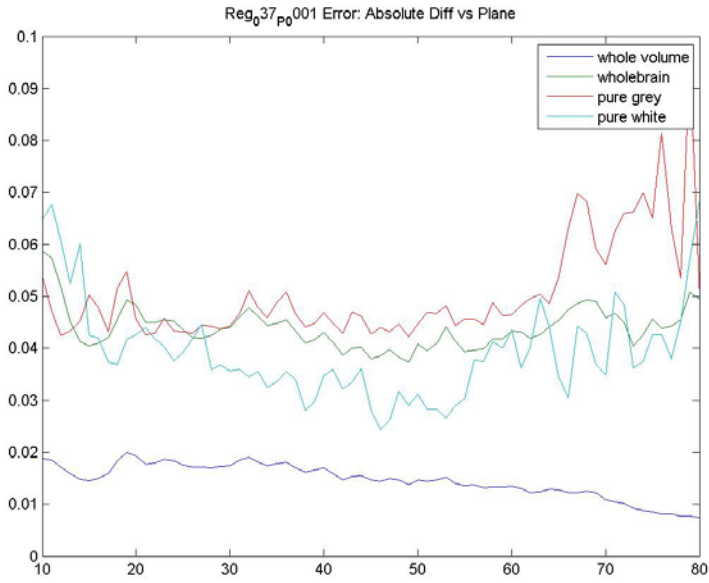


2517

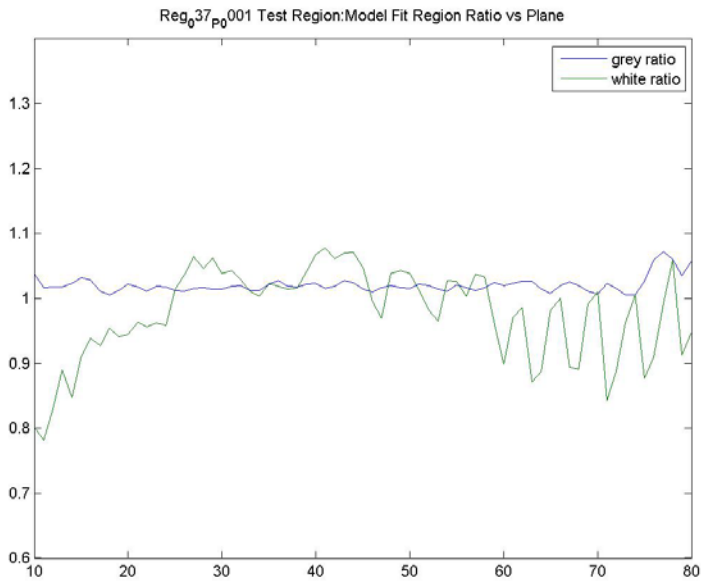


2518

2519


2520 Example #2. Another example of a good quality scan. ECAT HR+ (006_P_0001)

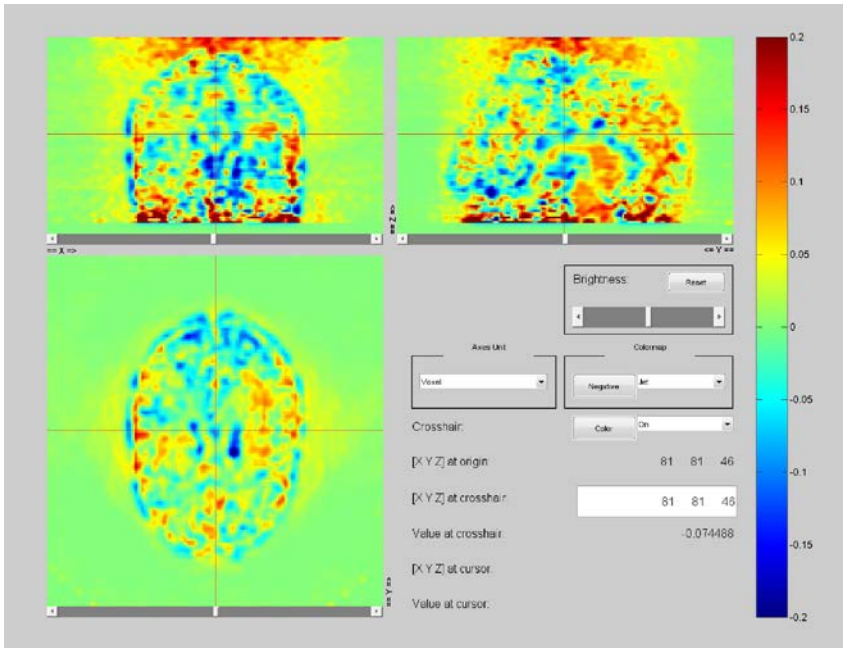


2521
2522

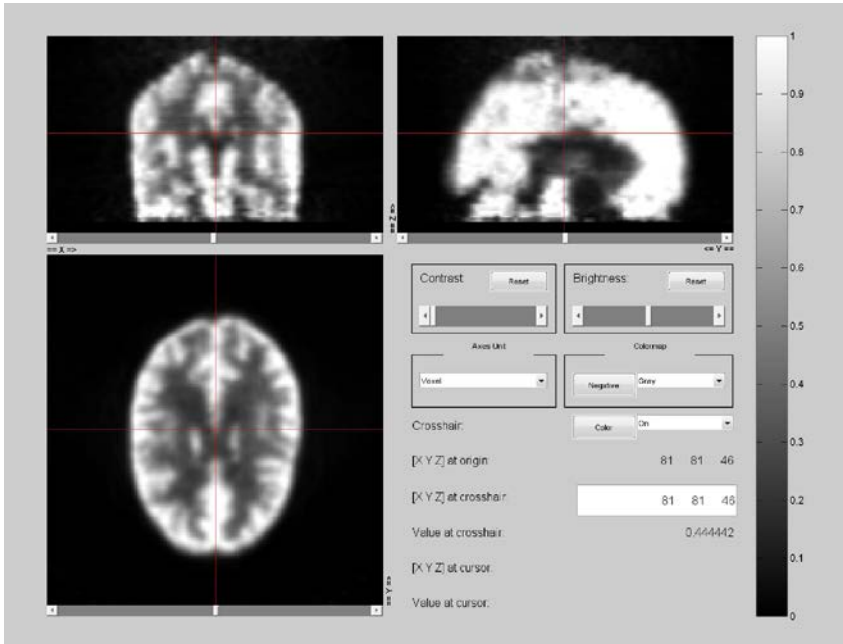

2523

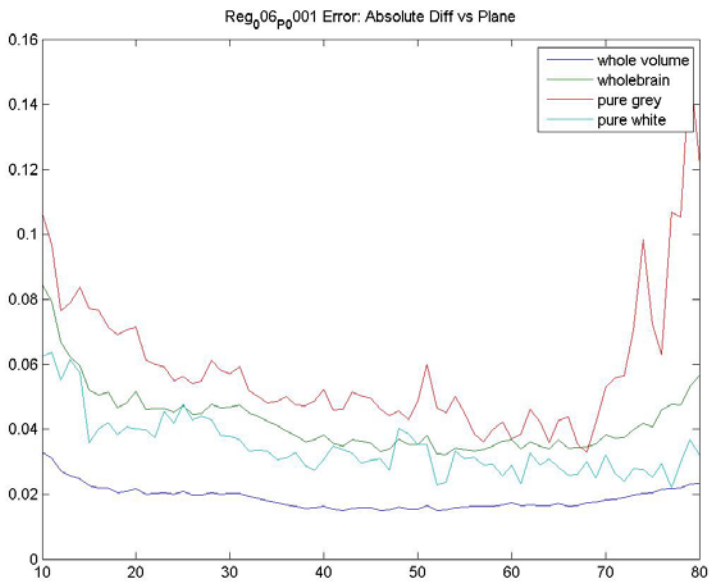


2524
2525

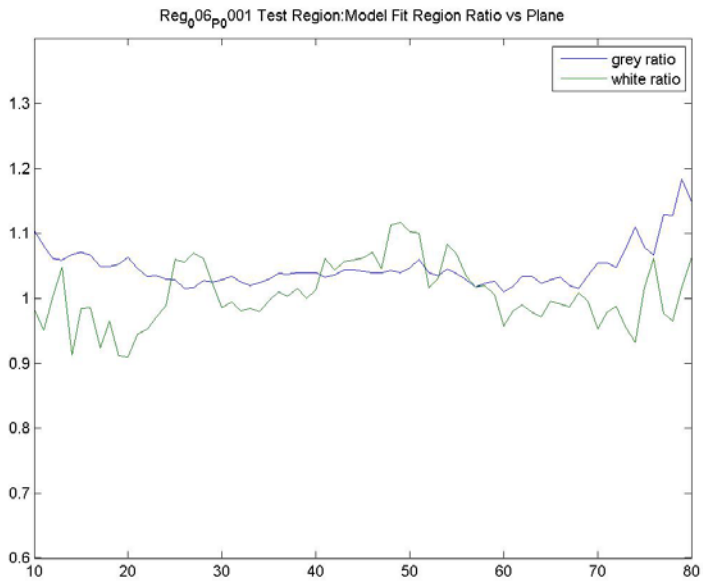


2526
2527

2528
2529
2530


Example #3. Siemens ECAT Accel (098_P_0002). Example with relatively poor image quality. Asymmetry seen between left and right side, and large errors between planes 30 and 50. But is this a function of poor scan quality, or a Hoffman phantom with extra space between plexiglass planes?

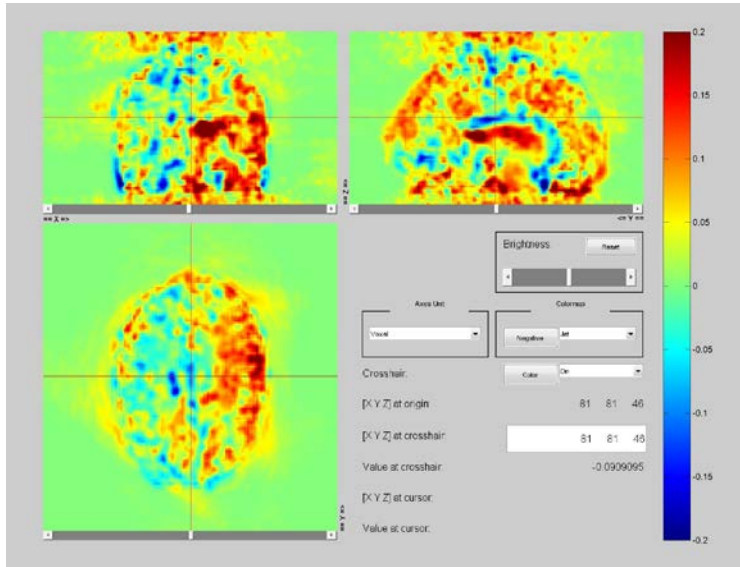


2531
2532

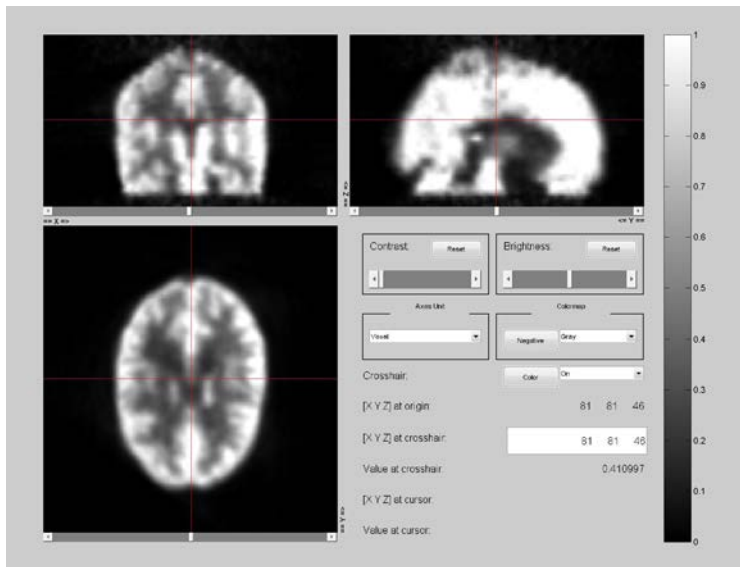

2533

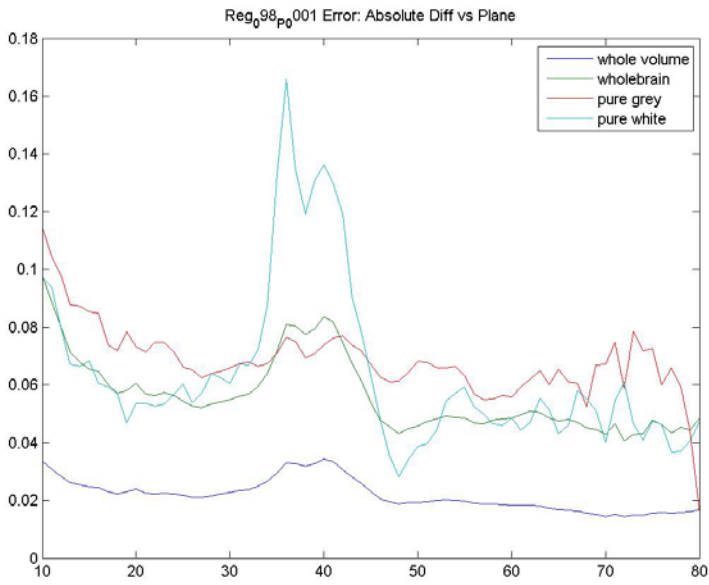

2534

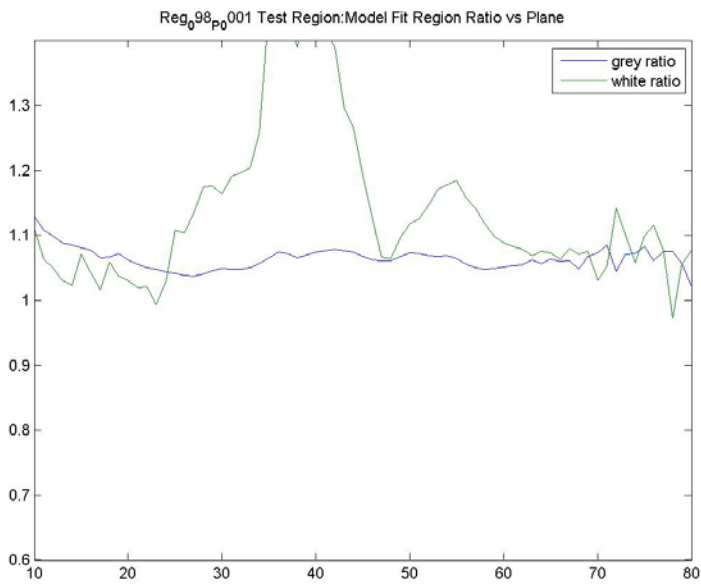


2535


2536

2537
2538
2539


Example #4. HRRT Example (128_P_0001). Poor performance at bottom of volume most likely due to scatter correction problems. Otherwise, the scan quality is reasonably good. Difference image for most of the brain is negative (blue regions) probably due to global image intensity normalization been driven too low by the high intensities seen in the lower planes.

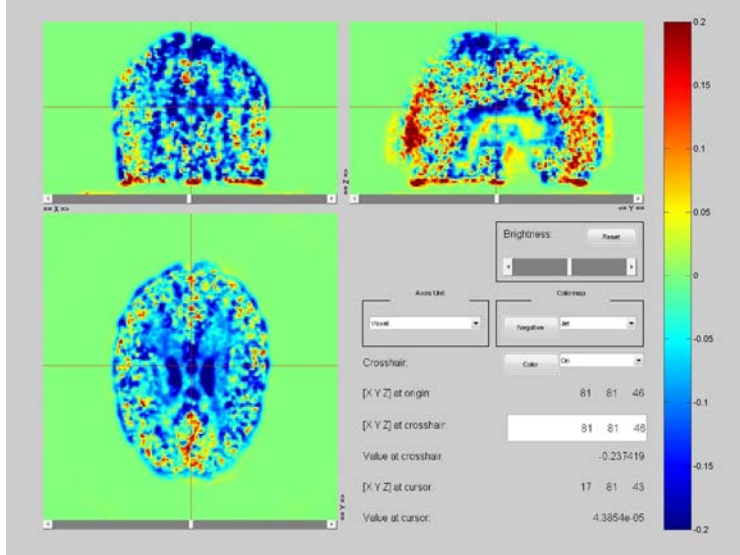


2540
2541

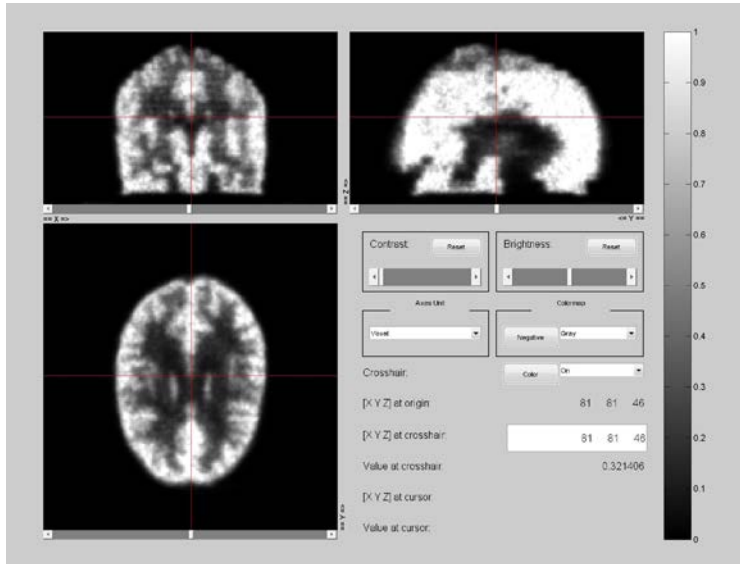

2542

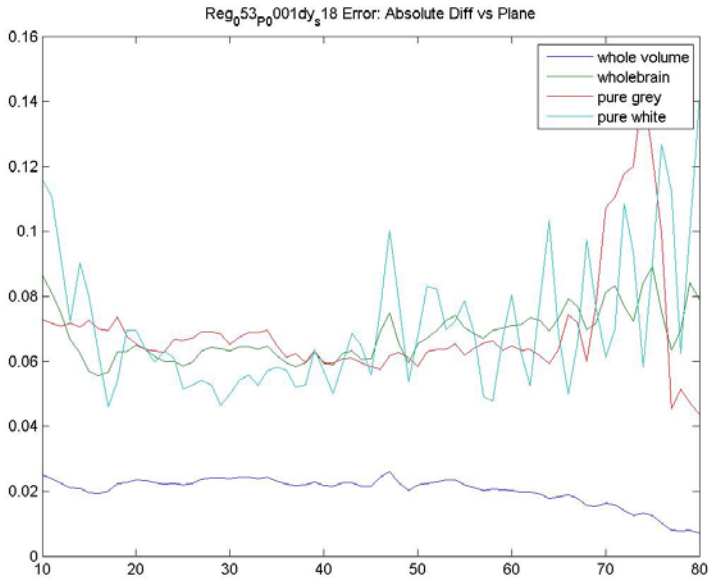

2543

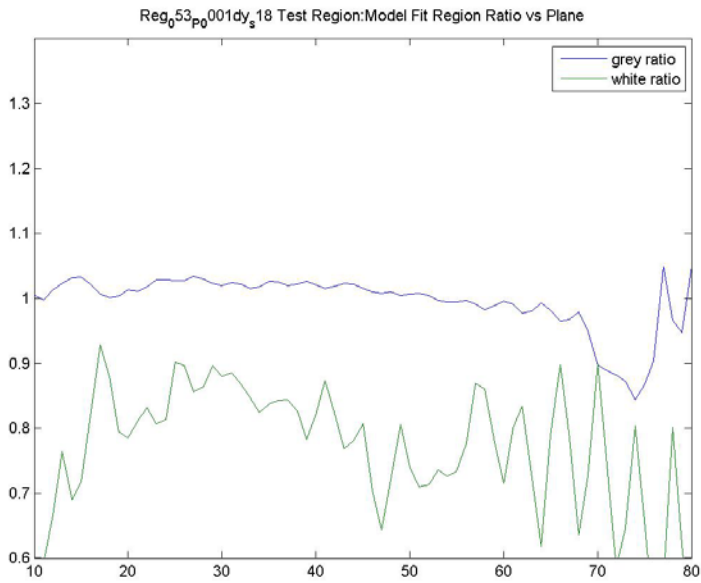


2544


2545

2546
2547


Example #5. (136_P_0004) – GE Discovery ST. Poor Quality – likely fail. Very large errors in the frontal lobe regions. White matter values compared to reference very high.

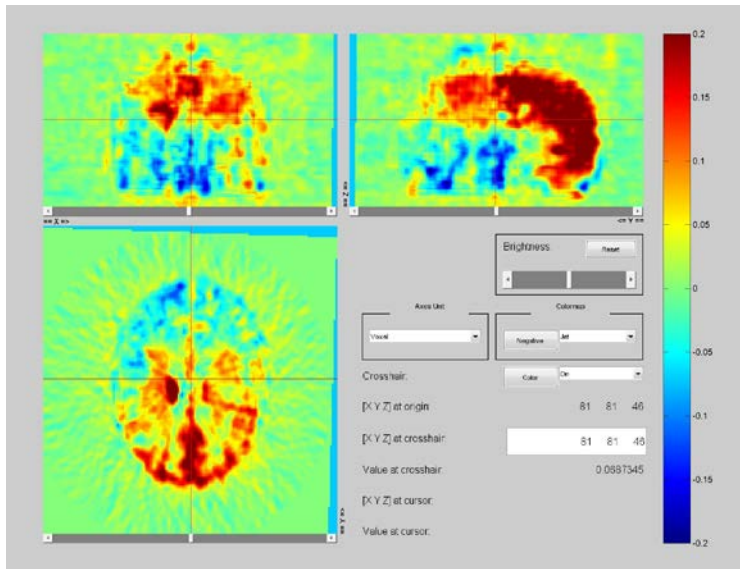

2548
2549

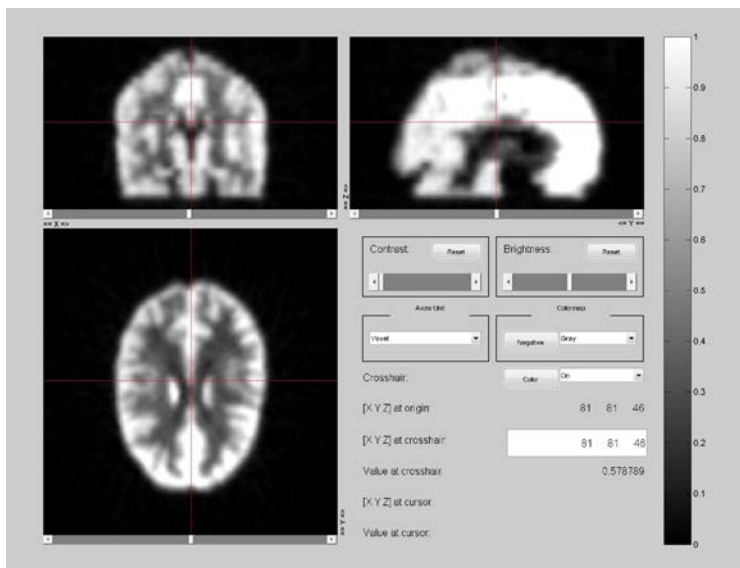

2550

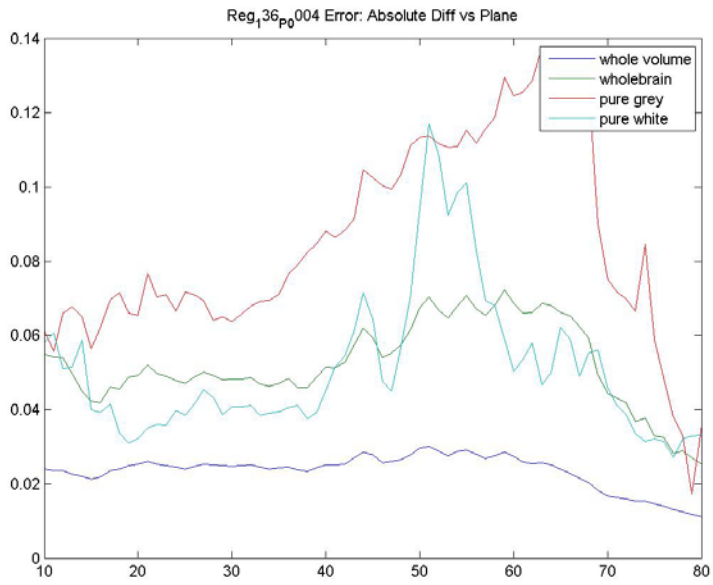

2551
2552
2553
2554

2555 **Appendix I: Kinetic Modeling and Comparison to SUVR**

2557 This section is intended as a reference to explain (a) the difference between late timeframe SUVR
 2558 measurement and the DVR measure calculated through full kinetic modeling, (b) reasons that amyloid
 2559 burden values can differ between these two approaches, (c) cautions regarding potential sources of error
 2560 introduced in SUVR measurement that are addressed through kinetic modeling, (d) logistical considerations
 2561 in acquiring full dynamic images, and (e) recommendations for measurement approaches.

2562 **The contributors to amyloid PET signal**

2564 The signal intensity measured in a particular image voxel (three dimensional pixel) of a PET image reflects
 2565 the amount of radiotracer present in that location at the time of measurement. To translate the signal
 2566 intensity of an amyloid PET tracer into a meaningful measure of amyloid binding, it is necessary to separate
 2567 out the contributions of tracer present in the blood, tracer bound to the target (the measurement of
 2568 interest), tracer bound non-specifically (to entities other than target, for example white matter) and
 2569 unbound tracer in tissue. The amount of tracer in each of these is dependent upon blood flow rate,
 2570 membrane permeability impacting the rate of tracer diffusion into tissue, the presence of target (e.g.
 2571 amyloid) in tissue, and the rate at which the tracer is cleared from the body ("clearance rate").

Signal intensity in first few minutes reflects perfusion

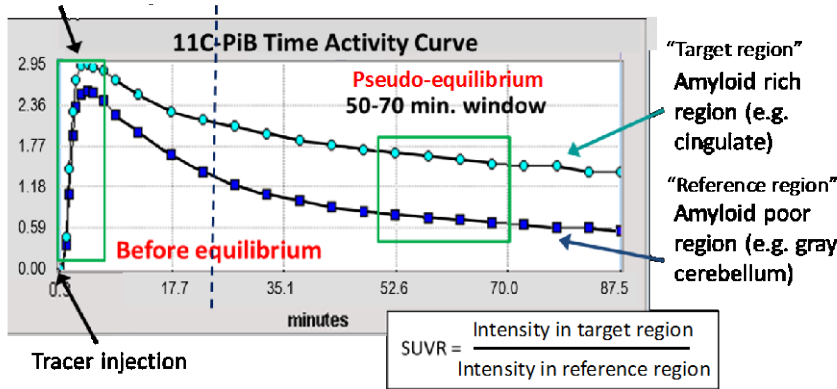


Figure 1.

2573 **Time activity curves.**


2574 **Stages of tracer uptake and clearance**

2577 Figure 1 shows the signal intensity measured for the original amyloid tracer 11C-PIB in two different regions
 2578 of the brain from the time of tracer injection to 90 minutes post-injection. The signal intensity curve for any
 2579 given region over the time from tracer injection to a time following achievement of relative equilibrium is
 2580 called a Time Activity Curve (TAC). In the initial minutes, the signal intensity reflects the rate at which the

Formatted: Space After: 0 pt

2581 tracer is being taken up into tissue (perfusion multiplied by first pass extraction), which is driven by the
2582 combination of blood flow rate and membrane permeability. Studies of amyloid tracers including 11C-PIB
2583 and Amyvid (florbetapir) have demonstrated a strong correlation between the early frame image and that
2584 of a blood flow image for the same subject (Forsberg 2012, Gjedde 2013, Hsiao 2012, Rostomian 2011).
2585 Following the first few minutes, the tracer begins to clear from the tissue, clearing less rapidly from
2586 amyloid-containing tissue to which the tracer binds. The rate of clearance into the bloodstream and out of
2587 the body is determined by several factors including kidney function and medication effects. After a tracer-
2588 specific period of time (40 to 45 minutes for 11C-PIB), the rate of tracer influx to tissue is in approximate
2589 equilibrium with its efflux back to the bloodstream.

2590
2591 Using the TAC values from Figure 1, the SUVR over time is shown in Figure 2. It can be noted that this SUVR
2592 is not a stable value over time, for reasons discussed below. For a visualization of SUVR over time using the
2593 amyloid tracer flutemetamol see also Figure 6 of Nelissen et al (2009).

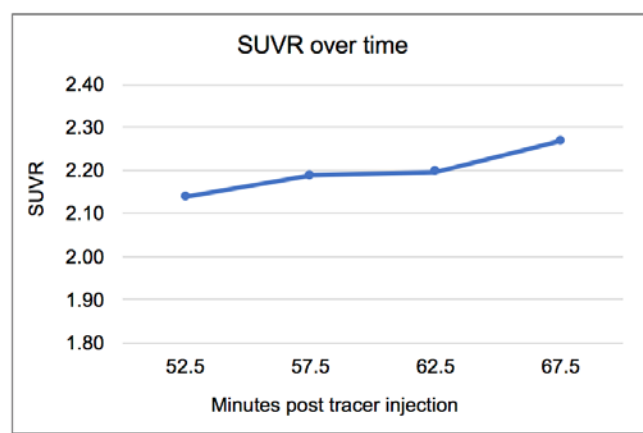

2594
2595
2596 Figure 2. SUVR over time based upon the TAC values in Figure 1.

2597 **Kinetic modeling**

2599 Several different models have been developed that use simultaneous differential equations to solve for the
2600 “flux” into and out of compartments, and ultimately the amount of tracer bound to target (in this case,
2601 amyloid). The gold standard approach uses arterial blood measurements to obtain the actual tracer
2602 concentration in blood. This method has some disadvantages due to patient and staff burden and variability
2603 in the blood measurements (Lopresti 2005, Tolboom 2009). Alternate modeling approaches make use of
2604 regional measurement of carotid artery radioactivity (Lopresti 2005) or eliminate the need for blood
2605 sampling by making use of reference measurements in tissue that does not contain the binding target. For
2606 amyloid tracers, this is often the cerebellar cortex, which is generally devoid of amyloid except in latest
2607 stages of Alzheimer’s disease (ref) and certain familial forms of AD (Sepulveda-Falla 2011). The validity of
2608 the reference region approach as an approximation for blood based modeling must be tested for each new

Formatted: Space After: 0 pt

2609 tracer, as it has been for 11-PIB (Price 2005), Amyvid (florbetapir, Wong 2010), Vizamyl (flutemetamol,
2610 Nelissen 2009), and Neuroseq (florbetaben, Becker 2013). All kinetic models make use of the entire time
2611 course of tracer measurement (TAC) from time of injection to a point at which a “pseudo-equilibrium” has
2612 been reached. All of these models have the advantage of segregating the contribution of blood flow and
2613 clearance from that of bound tracer. In the process, they provide a measure of “R1”, i.e perfusion relative
2614 to reference perfusion. Given the correlation between blood flow and cerebral glucose metabolism that
2615 exists in many cases, this provides an additional “FDG like” image reflecting neuronal function. The
2616 creation of a full TAC using an early time window and late time window has also been demonstrated
2617 (Bullich 2017). The measure of target burden (in this case amyloid) derived from a kinetic model is called
2618 the Distribution Volume Ratio (DVR or $V_{\text{tissue}}/V_{\text{nondisplaceable}}$), equal to non-displaceable Binding Potential
2619 (BPnd) + 1. Published studies that used kinetic modeling may state the DVR value or may alternatively state
2620 the BPnd value when stating amyloid burden.

2621 **Standardized Uptake Value Ratio**

2622 Despite the advantages provided by full kinetic modeling in accounting for contributions from blood flow,
2623 binding, and clearance, there are practical drawbacks. It is difficult for patients, particularly those with
2624 disease, to lie still in the scanner for the hour plus it may take to acquire a dynamic scan. Acquiring dynamic
2625 scans presents additional burden on staff, and starting the scan at time of injection may require two
2626 technicians to be present. Historically, not all scanners have supported the acquisition modes or memory
2627 capacity required to acquire the number of discrete timeframes necessary to capture a full TAC, although
2628 most newer scanners have this capability. Using the scanner for a full hour or more also precludes its use
2629 for other patients during that entire time.

2630 For these reasons, the SUVR is often used as an approximation for DVR. This measurement uses only a “late
2631 timeframe” segment during which the tracer is in equilibrium. In true equilibrium, and assuming that blood
2632 flow rates are the same in target and reference tissue, the ratio of the two tissues provides a relative
2633 measure of the signal contribution due to amyloid binding. In reality, equilibrium is “pseudo”, in that tissue
2634 continues to lose activity. However, numerous studies have demonstrated that the simpler SUVR approach
2635 can provide discrimination between normal, MCI, and AD groups and, with adequate numbers of subjects,
2636 measure group level increases or decreases (Biogen ref) over time.

2637 **Bias in SUVR measurements**

2638 The fact that true equilibrium is never reached can create an upward bias in SUVR value relative to DVR
2639 (Slifstein et al, 2007, Carson et al, 1993, Frokjaer et al, 2007, van Berckel et al, 2013). To illustrate this
2640 conceptually, from the TACs in Figure 1, it can be seen that the “receptor poor” reference region TAC
2641 asymptotes, or flattens, more rapidly than the “receptor rich” TAC. This is because tracer binding slows
2642 tracer flux back into the bloodstream. Even in late timeframes, neither curve is flat, which would be the
2643 case if equilibrium were reached and net flux were zero. However, the receptor poor curve approaches a
2644 “flatter” stage first, as the concentration difference between tissue and plasma is lower. The difference
2645 between the rate of change in the receptor rich TAC (the SUVR numerator) and the reference TAC (the
2646 SUVR denominator) creates an artificially high value. A mathematical expression of this is provided in
2647 Slifstein et al (2007), which the reader is encouraged to review for further detail along with other
2648 references cited. In brief, as described mathematically in Slifstein, a change in concentration in a given
2649 region is depicted by $[k_1 * C_{\text{plasma}}] \text{ minus } [k_2 * C_{\text{tissue}}]$, where k_1 is the transport coefficient from plasma to
2650 tissue, C_{plasma} is the concentration in plasma, k_2 is the transport coefficient from tissue to plasma, and C_{tissue}
2651 is the concentration in tissue. At equilibrium, these would sum to zero consistent with a lack of net
2652 flux.

concentration change. The expression $C_{\text{tissue}}/C_{\text{reference}}$, which is the SUVR, would equal the DVR (where $DVR = V_{\text{tissue}}/V_{\text{ND}}$ and ND refers to nondisplaceable binding in reference region). However, only “pseudo-equilibrium” is reached and instead, $C_{\text{tissue}}/C_{\text{reference}} = [V_{\text{tissue}} * (k_1 C_{\text{plasma}} + |dC_{\text{tissue}}/dt|)] / [V_{\text{tissue}} * (k_1 C_{\text{plasma}} + |dC_{\text{reference}}/dt|)]$. The rate of change in tissue $|dC_{\text{tissue}}/dt|$ in the numerator of this expression is greater than the rate of change $|dC_{\text{reference}}/dt|$ for the reference tissue (which “flattened” earlier) in the expression denominator. This erroneously increases the value of the $C_{\text{tissue}}/C_{\text{reference}}$, the SUVR.

SUVR bias is often on the order of 10% (Lopresti 2005) but can reach 20% or greater depending upon the value of k_1 (van Berckel et al, 2013). Bias increases from the point at which the approach toward pseudo-equilibrium begins (e.g. 30 to 35 minutes for 11C-PIB) and continues to increase (until approximately 70 minutes for 11C-PIB, van Berckel et al, 2013) before plateauing. If blood flow and clearance rates do not change from scan to scan, this bias would cancel out for longitudinal measurement. However, longitudinal error in measuring a change in SUVR can occur if the k_1 value changes from one scan to another. Changes in k_1 are influenced by blood flow and first pass extraction. Blood flow in particular can be impacted by medications including candidate therapeutics for AD. In a simulation modeled by van Berckel et al, error decreases with later timeframes, but for a decrease in k_1 from 0.32 to 0.26 the error introduced at 60 minutes would be approximately -4%, significant in the context of amyloid accumulation rates.

Longitudinal error can also occur if the ratio (R1) of the rate of tracer delivery to the target (“amyloid rich”) region to the rate of tracer delivery to the reference region changes from one scan to another. Such a change could be produced by (a) blood flow rate changes (e.g. decreases) in certain cortical regions relative to flow rate in a cerebellar reference region, or (b) changes in regional membrane permeability influencing tracer extraction efficiency. Using a longitudinal follow up period of 30 +- 5 months, Van Berckel et al found that R1 values were stable over time in normal controls and MCI patients, but were reduced by approximately 20% in AD patients. This is consistent with decreases in blood flow that have been observed with AD progression in regions consistent with those in which glucose hypometabolism becomes pronounced. Changes in regional blood flow rate and local membrane permeability can also be caused by therapeutic agents. A 20% reduction in R1 value was estimated to create a 2% longitudinal increase in SUVR at 60 minutes post tracer injection (van Berckel). A study that used the early (first 20 minutes) and late frames (50 to 70 minutes) of florbetapir images acquired in ADNI subjects to estimate the contribution of blood flow unaccounted for in SUVR measures, also found that potential longitudinal errors on the order of 2% to 5% could occur in late MCI/AD patients due to changes in blood flow (Cselenyi et al, 2015). In the van Berckel example (Figure 1 of the reference publication), it can be seen that the error is more pronounced in the 60 to 90 minute SUVR than the 40 to 60 minute SUVR. While part of this may be due to the bias phenomenon, it has also been observed that 60 to 90 minute PIB SUVR measurements involve substantially more technical variability than earlier measurement, likely arising from lower tracer signal with noise inflated through decay correction, and greater subject motion as time in scanner proceeds.

Bias in kinetic models (and SUVRs) that use a reference region

It should be noted that bias also occurs in kinetic models, depending upon the model (and potentially the tracer) used, for a different reason than that discussed above for SUVRs. All reference tissue models, whether DVR or SUVR assume that:

1. the level of non-specific binding is the same in target and reference regions
2. the ratio $K1/k2$ is the same for target and reference regions.

If either of these assumptions is violated, then the reference tissue model will not produce a true reflection of binding to target. Whether or not the model can still be used on a practical basis depends upon study objectives. Assumption 1 could be violated in the case of off-target binding, which is not homogeneous, and assumption 2 could be violated in the case of blood brain barrier (BBB) breakdown.

In a comparison of several modeling methods applied to the same 11C-PIB scans, Lopresti et al (2005) compared DVRs generated using the Logan graphical model with arterial blood sampling over 90 minutes ("gold standard") to DVRs generated using methods including arterial sampling and a 60 minute interval Logan reference region models with cerebellar cortex as reference, the Simplified Reference Tissue Model (SRTM), and SUVRs measured from 40 to 60 minutes and 40 to 90 minutes with cerebellar cortex as reference. Logan reference tissue models showed a negative bias averaging -11% for high DVR subjects, while the SRTM model showed a mean 5% bias but with broader variance than all other models for low DVR subjects, and a mean -5% bias for high DVR subjects. For comparison, the mean bias for SUVR models, high DVR subjects was 6% (60 minutes) to 9% (90 minutes). Van Berckel et al (2013) showed that DVRs generated using the Logan reference region method were 6% lower than those generated using the model Receptor Parametric Mapping (RPM2), while SUVRs were biased upward. Kinetic model bias has been attributed to a suspected difference between tracer clearance rate in the cerebellar cortex reference tissue vs. plasma (Lopresti 2005), or to differences in model susceptibility to reference region noise (van Berckel 2013). These factors can be mitigated in part through optimized model selection.

Logistical considerations for dynamic modeling

Acquisition of discrete timeframe data for dynamic modeling requires several short duration frames occurring immediately following tracer injection, followed by longer timeframes later on. The scanner must be capable of acquiring multi-frame data and must have adequate memory storage to support what will likely be more than 20 frames in a single session (this issue has decreased with newer scanners). The site must also either have scanner equipment that provides for a button enabling start of scan along with tracer injection, or a second staff person available to initiate scanner data acquisition at time of injection. There are further considerations with the length of the IV line depending upon the tracer (due to affinity for tubing walls for some tracers), and the position of the subject within the scanner. As additional considerations, scanner utilization time and patient burden are increased. A dual "early" (first minutes post injection) and "later" (pseudo equilibrium) data acquisition approach has been demonstrated that allowed extrapolation of a full TAC for kinetic modeling while also allowing the subject to have a "break" (Bullich 2017). However, the potential benefit of allowing a site to fit an extra scan within that "break" period is offset by the potential occurrence of a delay in continuing the scan, and associated introduction of technical variability. To assess blood flow changes, alternate modalities such as arterial spin labeling (ASL) MRI have been proposed; however, these require validation for use in this context and do not capture clearance changes.

It should be noted that kinetic modeling does not overcome error introduced by subject motion, misalignment between emission and transmission scan, or other technical sources of noise. Since the risk of subject movement increases with longer times in the scanner, these variables can actually outweigh the benefits unless provisions are made to align each timeframe prior to attenuation correction.

Conclusions

Longitudinal changes in SUVR arising from systematic changes in blood flow ratios and clearance rates mentioned in this section are not accounted for in the coefficient of variation in the profile Claim, which

2745 captures non-systematic variability. The impact of systematic changes is highly dependent upon the study
2746 population and therapeutic agent. When evaluating patient populations where the disease process may
2747 impact blood flow or clearance rate, or where a therapeutic intervention could impact these factors, it is
2748 strongly recommended to conduct at least an initial study using full dynamic modeling in order to
2749 determine whether the SUVR approach is an acceptable substitute. Despite the logistical challenges of
2750 conducting full dynamic imaging, there are certain sites that routinely acquire data of this type. The benefit
2751 of characterizing potential erroneous signal changes due to changes in blood flow or clearance merits
2752 inclusion of such studies prior to broadening a longitudinal amyloid measurement trial through use of
2753 SUVR.
2754
2755